

(19) World Intellectual Property Organization  
International Bureau



(43) International Publication Date  
17 May 2001 (17.05.2001)

PCT

(10) International Publication Number  
**WO 01/35081 A1**

- (51) International Patent Classification<sup>7</sup>: **G01N 21/65**
- (21) International Application Number: **PCT/US00/42139**
- (22) International Filing Date:  
13 November 2000 (13.11.2000)
- (25) Filing Language: **English**
- (26) Publication Language: **English**
- (30) Priority Data:  
60/165,075 12 November 1999 (12.11.1999) US  
60/170,682 14 December 1999 (14.12.1999) US  
09/629,790 31 July 2000 (31.07.2000) US
- (71) Applicants: **THE PENN STATE RESEARCH FOUNDATION** [US/US]; 304 Old Main, University Park, PA 16802 (US). **NATAN, Michael, J.** [US/US]; 726 Casa Bonita Court, Los Altos, CA 94024 (US).
- (72) Inventors: **PENA, David**; 124 S. Sparks Street, State College, PA 16801 (US). **GOODRICH, Glenn**; 3181 Shellers Bend #5, State College, PA 16801 (US). **HE, Lin**; Apartment #70, 2650 California Street, Mountain View, CA 94040 (US). **LYON, L., Andrew**; 1675 Broussard Way, Marietta, GA 30066 (US). **MUSICK, Michael, D.**; 916 Southgate Drive, State College, PA 16801 (US). **HOLLIWAY, William, D.**; 1005 Treelodge Parkway, Dunwood, GA 30350 (US).
- (74) Agent: **MONAHAN, Thomas, J.**; The Pennsylvania State University, Intellectual Property Office, 113 Technology Center, University Park, PA 16802-7000 (US).
- (81) Designated States (*national*): AE, AG, AL, AM, AT, AU, AZ, BA, BB, BG, BR, BY, BZ, CA, CH, CN, CR, CU, CZ, DE, DK, DM, DZ, EE, ES, FI, GB, GD, GE, GH, GM, HR, HU, ID, IL, IN, IS, JP, KE, KG, KP, KR, KZ, LC, LK, LR, LS, LT, LU, LV, MA, MD, MG, MK, MN, MW, MX, MZ, NO, NZ, PL, PT, RO, RU, SD, SE, SG, SI, SK, SL, TJ, TM, TR, TT, TZ, UA, UG, UZ, VN, YU, ZA, ZW.
- (84) Designated States (*regional*): ARIPO patent (GH, GM, KE, LS, MW, MZ, SD, SL, SZ, TZ, UG, ZW), Eurasian patent (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM), European patent (AT, BE, CH, CY, DE, DK, ES, FI, FR, GB, GR, IE, IT, LU, MC, NL, PT, SE, TR), OAPI patent (BF, BJ, CF, CG, CI, CM, GA, GN, GW, ML, MR, NE, SN, TD, TG).
- Published:**  
— *With international search report.*  
— *Before the expiration of the time limit for amending the claims and to be republished in the event of receipt of amendments.*
- For two-letter codes and other abbreviations, refer to the "Guidance Notes on Codes and Abbreviations" appearing at the beginning of each regular issue of the PCT Gazette.*

WO 01/35081 A1

(54) Title: **BIOSENSING USING SURFACE PLASMON RESONANCE**

(57) Abstract: The invention provides methods and reagents for the enhancement of surface plasmon resonance (SPR)-based detection assays. The methods and reagents can be used in any molecular recognition assay that uses a solid support. The invention also provides an SPR instrument that operates in imaging mode.

**BEST AVAILABLE COPY**

5

## BIOSENSING USING SURFACE PLASMON RESONANCE

## FIELD OF THE INVENTION

The present invention relates generally to surface plasmon resonance sensors. In particular, the present invention relates to instruments, methods and reagents for  
10 amplifying the surface plasmon resonance response and increasing its sensitivity, flexibility, throughput, specificity, and scope.

## BACKGROUND OF THE INVENTION

Surface plasmon resonance (SPR) is a general spectroscopic method for sensing refractive index changes near the surface of a metal film. Its sensitivity to these changes provides a versatile platform for the observation and quantitation of chemical reactions at the metal/solution interface, provided the chemistry is well-designed. The generality of the technique has led to its application to a variety of chemical systems, including biosensing (where specifically designed commercial instrumentation is available).

SPR allows detection of small changes in refractive index that result from interactions between surface-confined biomolecules and solution-borne species. For example, immobilization of a protein to the sensor surface allows for detection of protein binding events manifested by a change in refractive index and hence a change in the angle-dependent reflectance of the metal film. This type of SPR sensing is typically carried out on commercial instruments that use a carboxylated dextran gel on a Au film as the sensor surface, where the gel acts as a host for the surface-confined binding partner. However, SPR has been applied in a number of other formats, including imaging SPR where a large number of chemistries can be rapidly interrogated simultaneously. Likewise, a variety of other surface chemistries have been used as scaffolds for measurements of biomolecular interactions.

SPR relies on the optical excitation of surface modes (plasmons) in a free electron metal (e.g., a 50 nm thick film of Au, Ag, Al, or Cu anchored to a glass substrate by a thin adhesion layer of Ti, Cr, or mercaptosilane). Back-side, *p*-polarized illumination of a prism-coupled film at some angle greater than the critical angle for total internal reflection results in plasmon excitation at the metal-solution interface. Plasmon excitation is

observed as an increase in optical absorbance (decrease in reflectance) at an optimal coupling angle. This, in turn, results in a minimum in the SPR profile (a plot of reflectance versus angle), which is referred to as the plasmon angle ( $\theta_p$ ). Sensing via SPR is possible due to the sensitivity of  $\theta_p$  to changes in the index of refraction near the metal surface. Adsorption, desorption, and molecule-molecule interactions that occur at the metal-solution interface result in such changes, thereby inducing a shift in plasmon angle. These changes can be monitored in real-time, making SPR suitable for dynamic sensing.

Perhaps the most widely studied subset of chemistries using SPR is protein-protein interactions, where binding event signal transduction is difficult or impossible to accomplish by traditional optical spectroscopies. In order to decrease nonspecific binding and to increase surface loading of biomolecules, SPR experiments conducted on commercial instrumentation commonly use an extended coupling matrix in conjunction with the sensing surface. Such measurements typically begin with one protein immobilized on proprietary substrates comprising a carboxylated dextran (or "extended coupling") matrix layered on top of a thin evaporated Au film (i.e., between the film and the sample). The result is an extended three-dimensional array of molecules extending some 200 nm away from the surface of the Au film. Protein binding events leading to small changes in the refractive index of the dextran layer are detected via correspondingly small changes in the angle-dependent attenuated total reflectance. Despite the signal amplification afforded by the dextran matrix, the detection of small (<1000 MW) molecules is still a non-trivial task for commercial instrumentation. In some cases even the detection of species in the 2,000-10,000 MW range can prove challenging.

Use of coupling matrices is associated with a number of additional drawbacks, including the possibility of nonspecific interactions with biomolecules that dominate the signal, and the exclusion of large proteins. Furthermore, improper orientation of biomolecules within the matrix often leads to low biomolecular activity, especially with proteins. Because mass transport to molecules immobilized in the matrix is commonly pH dependent, separate steps are required to optimize diffusion of reagents into the matrix during the assay. These shortcomings can create significant difficulties in assay design. It would be desirable to avoid these problems by using planar SPR substrates (i.e., without an overlying matrix) such as Au films modified with a monolayer of a bifunctional organic

crosslinker. However, SPR reflectivity changes within these more uniform substrates are often too small to be measurable in any practical assay.

The applicability and usefulness of SPR could be greatly expanded if ligand binding events resulted in more pronounced changes in refractive index and, hence, more pronounced shifts in plasmon angle. Such increased sensitivity could make the technique  
5 broadly applicable to high-throughput screening of low molecular-weight drug candidates.

It is an object of the present invention to provide instruments, methods and reagents for the amplification of SPR reflectivity changes in chemical assays, especially in biomolecular recognition assays on planar SPR substrates coated with a monolayer or  
10 submonolayer of capture reagents (e.g., antibodies). It is also an object of the invention to provide methods and reagents for ultra-sensitive, non-PCR-based DNA detection assays. It is moreover an object of this invention to describe an SPR-based method for measuring distances between surface-confined objects on the scale from 1 to 500 nm, with 3-Angstrom resolution.

15 An additional object of this invention is to enable high throughput screening reactions (both primary and secondary) by amplified imaging SPR.

A further object of the invention is to provide a "wet chemistry" method for the synthesis of Au films for SPR (or other surface spectroscopies) as a replacement for (or alternative to) cumbersome evaporative methods used in the art.

20 Finally, it is an object of the invention to provide an imaging SPR instrument capable of depicting spatial differences in film reflectance at fixed angles of incidence, which spatial differences are induced by differential indices of refraction or film thickness (i.e., differential chemical modification). The imaging SPR instrument provided by the invention allows SPR to be used in multiplexed biological "chip" assay formats. For  
25 example, the imaging SPR instrument would be integral in the simultaneous detection of multiple target analytes using a solid support to which ligands for the different target analytes are attached at specific locations.

The instrumentation, methods, and reagents of the present invention enable chemical assays (including multiplexed biosensing assays) of unprecedented sensitivity  
30 and selectivity.

## SUMMARY OF THE INVENTION

The present invention provides instrumentation, methods, and reagents for the amplification of SPR reflectivity changes. In one series of embodiments, colloidal-metal nanoparticles are used as optical tags for SPR-based sensing assays. These embodiments  
5 rely on the observation that the SPR response of a metal film changes dramatically upon localization of such colloidal-metal nanoparticles to the film surface. The dramatic change in the SPR response of metal films that occurs upon adsorption of colloidal metal nanoparticles can be exploited in any assay that depends on the occurrence of a molecular recognition event (e.g., the binding of antigen to an antibody, the binding of a ligand to its  
10 receptor, or the hybridization of complementary nucleic acid molecules). In one of the many possible implementations, one of the molecules that participates in a molecular recognition event is immobilized on the surface of a metal film of the SPR substrate (or to an entity attached to the metal film). Another molecule that participates in the interaction with the immobilized molecule – either by binding directly to the immobilized molecule,  
15 or by binding to a third molecule that in turn binds to the immobilized molecule – is then tagged with the colloidal metal nanoparticle. The binding between the participating molecules leads to colloidal metal adsorption, with the concomitant change in the SPR response of the film. Methods are well known in the art for preparing monodisperse colloidal metal nanoparticles in solution, as are methods for attaching biomolecules to the  
20 metal nanoparticles without loss of biological activity. In some embodiments, the use of colloidal Au nanoparticles leads to a 100,000-fold increase in SPR sensitivity.

For example, colloidal Au nanoparticles can be readily attached to ligands of target analytes. Then, when the target analyte becomes localized to the surface of the SPR film (or to ligands immobilized thereon), the Au-tagged ligands are brought to the surface  
25 when the ligands bind the target analyte, leading to the amplified changes in SPR reflectivity. The amplification in signal is sufficiently large that planar SPR substrates (such as a Au film modified with a bifunctional organic cross linker) can be used, thus avoiding several of the problems associated with commercial dextran-based matrices.

Notwithstanding the significant limitations discussed above, dextran-based SPR  
30 substrates are adequate for some types of assay. For this reason, the invention also provides methods for the amplification of SPR reflectivity within dextran-based matrices. In some embodiments of the invention, Au nanoparticles attached to ligands are first

brought to the matrix and retained there through the biomolecular interaction that forms the basis of the assay. The nanoparticles are chosen to be of a sufficiently small diameter to permit efficient diffusion into the network. However, nanoparticles of this size do not optimally amplify changes in SPR reflectivity. Consequently, to optimize amplification, the nanoparticles are then enlarged through addition of an Ag plating solution.

In other embodiments, the invention provides a method for further enhancing colloidal Au-amplified SPR reflectivity by overlaying an inorganic film over the Au surface. The distance between the metallic nanoparticles and the metal surface has a significant impact on SPR reflectivity. In preferred embodiments, a 30 nm thick film of SiO<sub>2</sub> is evaporated onto a 50 nm Au surface. When colloidal gold nanoparticles become attached to this surface – either directly or by way of, e.g., a protein-protein interaction – the SiO<sub>2</sub> layer acts as a spacer to optimize the coupling distance between the Au nanoparticles and the Au surface. This leads to a greater shift in the plasmon angle (i.e., angle of minimum reflectance) than observed using colloidal Au nanoparticles and a Au surface without an SiO<sub>2</sub> film. The enhancement is observed even when the Au surface is bound to very low levels of colloidal Au (e.g., less than 1% surface coverage).

In another series of embodiments, the methods are used to provide a “sandwich” immunoassay. Specifically, a primary “capture” antibody to a target analyte is immobilized on the surface of an SPR substrate, either on the Au surface itself, or on an overlaying SiO<sub>2</sub> film (or other material). A secondary antibody to the target analyte is conjugated to colloidal Au nanoparticles by one of a variety of methods. The Au nanoparticles and the SPR substrate are then contacted with a biological fluid suspected of containing the target analyte. If present, the target analyte will become bound to the SPR substrate through its interaction with the immobilized capture antibody, and the colloidal Au will become localized to the SPR substrate through the interaction between the secondary antibody and the bound target analyte. As a result, an amplified change in the plasmon angle will be observed, amplified with respect to the angle shift observed if the secondary antibody was not conjugated to colloidal Au nanoparticle. In some cases, the methods provided herein provide a 100,000-fold or greater enhancement in SPR signal relative to conventional SPR assays using dextran-based capture matrices, and provide the capability for detecting protein concentrations of less than 70 fM. It should be clear to those skilled in the art that such assays can be carried out in separate steps, in which the

analyte-containing solution is first exposed to the surface, and wash steps are carried out to eliminate non-specific binding. Then, in a second step, the colloidal Au:antibody conjugate is introduced.

In another series of embodiments, the methods of the invention are applied to  
5 detect target nucleic acid sequences. For example, a "first nucleic acid probe" may be immobilized on the surface of a planar SPR substrate and a "second nucleic acid probe" conjugated to colloidal Au nanoparticles. The probes have regions at least partially complementary to the target nucleic acid sequence (or are capable of some other interaction) such that in the presence of the target sequence, both the probes become  
10 associated therewith. As a result, the colloidal Au nanoparticles conjugated to the second nucleic acid probe become localized to the SPR substrate and there is an amplified plasmon angle shift. The methods of the invention enable a quantitation limit of better than  $8 \times 10^7$  molecules/cm<sup>2</sup> for a 24-mer oligonucleotide with approximately 5 decades of dynamic range. This is more than a 1000-fold improvement in the sensitivity observed  
15 without using the amplifying methods of the invention. In this embodiment as well, introduction of the second nucleic acid probe can occur before, at the same time, or after introduction of the target sequence.

The invention also provides an SPR instrument capable of operating in imaging mode rather than scanning mode. Scanning mode SPR measures a single SPR reflectivity  
20 value for the entire SPR substrate at each angle of incidence (and/or wavelength of the incident light) within a specified range. The imaging mode instrument uses a charge-coupled device (CCD) to provide an image that depicts local SPR reflectivity values throughout an SPR substrate at one or more predetermined angles of incidence. The angle(s) of incidence chosen is the angle at which the largest change in SPR reflectivity is  
25 observed upon occurrence of the event to be assayed (e.g., upon the binding of an immobilized ligand to its target). This enables SPR to be used as the basis for detection in microarray format for the purpose of multiplexed assays. In such assays, the SPR instrument captures a normalized reflectance image of the SPR substrate after addition of the fluid suspected of containing the target analyte. In the resulting image, the intensity of  
30 the reflectance signal in each "spot" on the substrate yields information about the amount of target analyte present at that location. The imaging SPR apparatus described herein allows for the simple introduction of large samples (up to 50 mm x 50 mm microarray

substrates, using commercially available optics). Moreover, with custom optics, much larger surfaces, e.g., 6 inches x 6 inches, can be used. Unlike previously described SPR instruments, the imaging device of the present invention provides a unique horizontal sample geometry that enables the robotic manipulators to control substrate handling and liquid delivery. This geometry obviates the need to flow solutions onto a vertical SPR substrate, as is required in prior art instrumentation.

Modifications to particles and/or surfaces aimed at increasing sensitivity and selectivity of SPR include the use of: (i) new types of metal nanoparticles such as AuS/Au core-shell particles, designed to optimize the wavelength-dependent component of dipolar coupling to surfaces; (ii) particles with sophisticated surface functionalization that exhibit reduced non-specific binding and that allow control over the number of biomolecules bound to the particle; (iii) substrates with sub-wavelength holes designed to provide local field enhancement; and (iv) oxide-coated metal films that optimize the distance dependent component of particle-surface coupling. Instrumental approaches to increased sensitivity include the use of tuned excitation wavelengths, measurement of angle-dependent surface plasmon scattering in parallel with SPR, and interferometric SPR. A third line of embodiments to improve SPR sensitivity involves the use of two secondary signal amplification schemes. One is based on particle "development", in which selective chemistries are used to grow the dimensions of immobilized particles; a second is based on a cascade effect in which molecular recognition-induced binding of one metal nanoparticle leads to selective deposition of several others from solution.

To define regions of the SPR substrate for different chemistries, a method has been developed for producing disposable replicas of printed circuit boards. The resulting "nanobeakers" (fabricated from polydimethylsiloxane, or PDMS) allow the ability to individually address a large number of spatially distinct regions over a small surface. Use of such microwell assays have illustrated that changes in Au particle coverage of less than 0.1 % of a monolayer are easily detected by imaging SPR.



## BRIEF DESCRIPTION OF THE DRAWINGS

FIGURE 1 illustrates the changes in the SPR profile of a 50 nm thick Au film SPR substrate that result from adsorption of 11 nm diameter colloidal Au nanoparticles.

FIGURE 2 illustrates how the SPR profile of a 47 nm thick Au film changes upon  
5 adsorption of colloidal Au nanoparticles of size 30 nm- 59 nm.

FIGURE 3 illustrates how the SPR profile of a Au film changes with different surface coverages of 35 nm (FIGURE 3A) and 45 nm (FIGURE 3B) colloidal Au nanoparticles.

FIGURE 4 illustrates differential SPR profiles (angle of incidence versus  
10 percentage change ( $\Delta$ ) in reflectance) for the data presented in FIGURE 3.

FIGURE 5 plots the maximum change in reflectance as a function of number density for colloidal Au nanoparticles 30 nm – 59 nm in diameter.

FIGURE 6 illustrates schematically an example of a sandwich immunosensing assay.

FIGURE 7 illustrates sandwich immunoassay SPR profiles obtained using an  
15 unconjugated secondary antibody (FIGURE 7A) and a secondary antibody conjugated to colloidal Au nanoparticles.

FIGURE 8 illustrates a differential SPR profile ( $\Delta$  % reflectance versus angle of incidence) for the data presented in FIGURE 7.

FIGURE 9 illustrates reflectance time courses for the immobilization of both the  
20 unconjugated and the Au-conjugated secondary antibodies.

FIGURE 10 illustrates the variation in colloidal Au induced plasmon shift at varying concentrations of target analyte in an immunosensing assay.

FIGURE 11 illustrates the progressive enhancements in SPR response that occur  
25 when a Au film is coated with a 15 nm (FIGURE 11A), 24 nm (FIGURE 11B), and 33 nm (FIGURE 11C) thick layer of SiO<sub>2</sub> and then has 12 nm colloidal Au adsorbed thereon.

FIGURE 12 illustrates schematically an example of a nucleic acid hybridization assay.

FIGURE 13 illustrates an SPR profile for a nucleic acid hybridization assay  
30 conducted using the scheme in FIGURE 12.

FIGURE 14 illustrates schematically an example of an imaging SPR instrument provided by the instant invention.

FIGURE 15A shows the SPR minimum for the following modifications on a mixed SAM (90% 11-mercapto-1-undecanol:10% 16-mercaptohexadecanoic acid/ on  
5 Au:electrostatically immobilized protein A/anti-IL-5 complex (a); 0.6 ng/mL IL5/25 mg/mL HAS (b); IL-5:Au (with 0.5% Blotto Blocker) (c). FIGURE 15B shows the SPR minimum in a similar experiment, but with 600 ng/mL/25 mg/mL HSA introduced.

FIGURE 16 shows the UV-Vis optical spectra of colloidal dispersions made by mixing  $\text{Na}_2\text{O}_3$  with HavCly in different ratios: (a) 1.3:1, (b) 1.2:1, (c) 1.4:1, and (d) 2.0:1.

10 FIGURE 17 depicts components of the fabrication process of PDMS microwell arrays from left to right: (A) the once inch square electronic breadboard "master", (B) the PDMS post "master", and (C) the PDMS well array replica of the electronic breadboard. The components were placed against a dark background to enhance the features formed from the colorless PDMS.

15 FIGURE 18 depicts time lapse photos of bromocresol blue in selected wells of the PDMS array: (A) Time = 0, (B) Time = 30 minutes, (C) Time = 60 minutes, and (D) Time = 24 hours.

#### DETAILED DESCRIPTION OF THE PREFERRED EMBODIMENTS

20 The present invention provides a number of detailed protocols for ultra-sensitive biosensing assays that are enabled by this generalized sensing scheme. However, to aid in the understanding of the invention, a detailed description is also provided of the enhancement of the SPR response observed with adsorption (via a molecular interaction) of colloidal metal onto the metal film of the SPR substrate. The following definitions are  
25 also provided:

By "SPR substrate" is meant any material in which the phenomenon of surface plasmon resonance can be observed (i.e., the optical excitation of surface modes (plasmons) in a free electron metal when coupled to a prism). In preferred embodiments, SPR substrates comprise free electron metal films deposited or seeded onto a glass  
30 surface. Free electron metals include, but are not limited to, Au, Ag, Al, and Cu. The invention also contemplates the use of alloys or mixtures of metals.

By "SPR reflectivity" (or "reflectance") is meant the modulation of the intensity of light reflected from a prism to which an SPR substrate has been coupled. SPR reflectivity is at a minimum when surface plasmons are excited in the SPR substrate. Depending on the angle of incidence, SPR reflectivity values can range from 0% to 100% of the original intensity of the incident illumination.

By "SPR profile" is meant the value of SPR reflectivity of an SPR substrate at various angles of incidence (or at various wavelengths of incident light). SPR profiles are often depicted graphically as a plot of SPR reflectivity versus angle of incidence (or versus wavelength of incident light). By "angle of incidence" is meant the angle at which light entering a prism encounters the face of the prism to which the SPR substrate is coupled.

By "prism" is meant any optical element coupled with the SPR substrate through which incident light is directed, e.g., a polished SF11 glass onto which a film of Au has been evaporated. The preferred prisms of the instant invention include triangular prisms, most preferably with a  $70^\circ - 70^\circ - 40^\circ$  geometry, and hemispherical prisms.

Many of the examples and embodiments herein describe the use of Au film and colloidal Au nanoparticles, but it is to be understood that any other metal (including alloys and mixtures of metals) with an SPR response is also contemplated by and within the scope of the invention. Likewise, although examples of the methods of the present invention described herein are often directed to biosensing assays, the methods are also applicable to other SPR-based sensing configurations.

An important aspect of the present invention is the ability to multiplex assays using the SPR techniques of the present invention. Spatial multiplexing (i.e. arraying) is made possible by the physical separation of reagents on the metal substrate. However, additional multiplexing can be achieved by altering characteristics of the metal nanoparticles. Variables include changing the size and composition of the metal colloidal nanoparticles. Such multiplexing is best interrogated using traditional SPR, where the reflectivity of a film (as well as scattering therefrom) can be rapidly measured at every angle of incidence. However, multiplexing can be carried out using imaging SPR, potentially in conjunction with both light reflectance and scattering, and ideally after the reflectivity is measured as a function of incident angle.

FIGURE 1 illustrates the changes in the SPR response that accompany colloidal Au adsorption to a Au film. To generate the SPR profile (reflectance as a function of

incidence angle), a 50 nm thick Au film was modified with the bifunctional organic linker 2-mercaptoethylamine (MEA). The thiol group of MEA binds to the Au film, leaving free amine groups exposed on the surface. The solid line trace shows a sharp plasmon minimum (minimum reflectance value) at an angle of 43.7°. When the Au film is exposed to a 17 nM solution of 11 nm-diameter colloidal Au for 1 minute, Au particles bind to the Au film via these free amine groups. As shown by the dotted line trace in FIGURE 1, this results in a significant increase in the minimum reflectance value, a broadening of the SPR profile, and a 0.2° shift in the plasmon angle.

Exposing the Au film to the colloidal Au nanoparticles for an increased period of time was found to increase the magnitude of these changes. Thus, a 60 minute exposure resulted in a plasmon angle shift of 2.6° (i.e., to 46.3°) with an increase in the minimum reflectance value by nearly 40% over that of the Au film without any localized colloidal Au nanoparticles (a "bare" Au film). This is illustrated by the dashed line trace in FIGURE 1. A more complete discussion of the materials and methods used to generate the SPR profile in FIGURE 1 are provided in Example 1.

These results resemble the dramatic shifts induced by thin carbon coatings evaporated onto Ag surfaces, where the strong absorptivity of the film induces a significant degree of plasmon damping. Without wishing to be bound by a single theory or mechanism, it seems likely that a similar absorptive damping process is responsible for the SPR changes due to Au-colloid adsorption, as these particles possess a nonzero imaginary dielectric component. A second possible, and non-exclusive, mechanism for damping involves the coupling of the localized surface plasmon of the colloid with the propagating plasmon in the Au film, a situation that is similar to effects observed at roughened Au films and other particle-modified films.

When the time course of the change in reflectance is monitored at the reflectance minimum, a >1% reflectance change is easily observed in the first 100 ms of colloid adsorption. The surface coverage at this time is roughly 0.1% of a close-packed monolayer. If it is assumed that the plasmon angle changes linearly with surface coverage (a reasonable assumption for low coverages), and an instrumental angular resolution limit of 0.005°, a 40-fold (0.2°/0.005°) decrease in surface coverage is detectable. Accordingly, 0.0025% of a monolayer of 12 nm-diameter colloidal Au ( $2.0 \times 10^7$  particles/cm<sup>2</sup>) is easily observable. As discussed below, even lower coverages are observable using larger

diameter Au colloid. The time course of change in reflectance as a function of time is shown in the inset to FIGURE 1.

The effect that colloidal Au adsorption has on the SPR response of a Au film substrate depends dramatically on the size of the colloidal nanoparticles. The solid line  
5 trace of FIGURE 2 shows the SPR response of 47 nm thick Au films coated with MEA and then subsequently coated with similar number densities ( $1.3 \pm 0.15 \times 10^9$  particles/cm<sup>2</sup>) of 30, 35, 45, and 59 nm diameter colloidal Au. Despite the relatively low number density, the SPR profile changes dramatically with particle size, as the minimum reflectance increases from 10% to 35% over a less than 2-fold increase in diameter.  
10 Indeed, for the largest particle size (59 nm), the SPR profile bears little resemblance to that of a bare evaporated film; the profile is very shallow and broad, without the well-defined plasmon minimum that is typically observed in SPR. A more complete discussion of the materials and methods used to generate the SPR profile in FIGURE 2 are provided in Example 1.

15 It is important to note that, while the number of colloidal Au particles per unit area is being held constant for the data shown in FIGURE 2, the fractional surface coverage is varying with particle size. In other words, an equal number of two different size particles will cover different geometric areas. Taking this into account, the fractional coverage of 30, 35, 45, and 59 nm diameter Au particles are 1.2, 1.6, 2.6, and 4.5% of a close packed  
20 monolayer, respectively.

FIGURE 3 shows the changes that occur in the SPR profile as a function of surface concentration (expressed as the number of particles/cm<sup>2</sup>) for 35 nm (FIGURE 3A) and 45 nm (FIGURE 3B) diameter colloidal Au particles. In the case of 35 nm particles, a low number density of particles induces relatively small plasmon angle shifts and reflectance  
25 changes. As the number density is increased, changes in the position and the magnitude of minimum reflectance become larger, eventually attaining a total plasmon shift of about 7° and a reflectance increase of >40%. Somewhat larger angle shifts are observed with respect to the 45 nm diameter colloid Au particles; the initial change in plasmon angle is significant and increases rapidly with increasing surface concentration. However, the  
30 shape of the SPR profile evolves much more rapidly in the case of the 45 nm particle, as a >30% reflectance is observed at the lowest surface concentration. The trend is similar for other sizes of colloidal Au particle – smaller perturbations are observed for 30 nm

diameter particles and much larger initial reflectance changes are observed for 59 nm diameter particles.

From a practical standpoint, it is not the gross perturbation of the profile that is important in an SPR sensing format but rather the maximum change (either an increase or decrease) that can be observed in either the plasmon angle shift or in the reflectance. It is evident from the data shown in FIGURES 2 and 3 that, at higher surface coverage, the SPR profile becomes rather too broad for accurate plasmon angle determination. Therefore, in preferred embodiments, it is more practical from both an instrumental and a sensitivity standpoint to measure the reflectance change at a single angle, despite the fact that the reflectance change itself may possess no clear physical meaning in terms of the interfacial dielectric properties.

In preferred embodiments, the selected angle at which to measure reflectance is the angle at which the maximum reflectance change occurs upon binding of the colloidal Au nanoparticle to the Au film. The maximum reflectance change can be determined by taking the difference between the SPR profiles of the Au-colloid-modified film and the unmodified film. FIGURE 4 shows the difference profiles calculated from the data shown in FIGURE 3. For both the 35 nm diameter particles (FIGURE 4A) and 45 nm diameter particles (FIGURE 4B), the maximum increase in reflectance is observed at 43.7°. This result suggests that the minimum of the SPR profile for the unmodified film is the optimal observation angle for the Au-colloid-modified film. The large size of reflectance changes observed here suggests that much lower surface concentrations may be detectable. Indeed, for 45 nm diameter particles, a number density of  $1.3 \times 10^9$  particles/cm<sup>2</sup> results in a reflectance change of 40%. Because current scanning SPR instrumentation is able to detect a change in reflectance of < 0.1%, it is possible to detect a 400-fold lower surface coverage ( $3 \times 10^6$  particles/cm<sup>2</sup>, equivalent to 0.0065% of a monolayer), assuming a linear SPR response at low coverage.

In FIGURE 5, the maximum change in reflectance is plotted as a function of number density for the 30 nm, 35 nm, 45 nm, and 59 nm diameter colloidal Au particles. For all particle diameters, the peak of the differential profile is approximately 43.7°, again indicating that the ideal observation angle is the same, independent of particle size. In terms of assay and sensing applications, this is a distinct advantage of particle enhancement, as the angle where the largest signal will be observed can be known prior to

performing an assay. This may, in some cases, eliminate the need for high-resolution scanning in order to determine the amount of immobilized material. Measurement of the percent reflectance at a specific angle may also be subject to less error, as determination of the absolute plasmon angle becomes difficult at higher surface coverage.

- 5           It should be noted that while the focus of this invention is on SPR, with other analytical techniques used to assist in characterization, the other techniques themselves can provide sensitive DNA detection. Thus, in the absence of significant non-specific particle binding, single nanoparticles are easily visualized by atomic force microscopy, field emission scanning electron microscopy, or by near field scanning optical microscopy.
- 10   If the required detection limits for DNA are not achieved by SPR, other techniques can be utilized.

#### Biosensing Assay Formats.

- One assay format that can be readily used with the methods of the invention is the
- 15   “sandwich” assay, well-known in the art. Sandwich assays are generally organized in the following way: Ligand *A*, immobilized on a solid support, can bind to target analyte *B*, which can simultaneously bind ligand *C*. When put into contact, a complex is formed on the solid support between *A*, *B*, and *C*. If ligand *C* is labeled with a detectable “tag” then the amount of target analyte *B* can be quantified by measuring the signal of the detectable
- 20   tag present on the solid support. It will be appreciated that there can be many variations on this basic scheme. The “target analyte” is any analyte that is the subject of an assay; preferred targets of the invention are biomolecules, including but not limited to nucleic acids, proteins, hormones, sugars, and metabolites. The “ligand” is any species capable of binding to a target; preferred ligands of the instant invention include, but are not limited
- 25   to, antibodies and nucleic acids. The sandwich assay configuration is commonly used in immunoassays where the “ligands” are antibodies directed toward the target analyte.

- FIGURE 6 illustrates an example of the sandwich format in which a first antibody against an antigen is immobilized on the surface of the Au film. A second antibody against the antigen is conjugated to colloidal Au nanoparticles. When brought into
- 30   contact, a complex is formed on the solid support between the first antibody, the antigen, and the second antibody conjugated to a colloidal Au nanoparticle.

FIGURE 7 shows data from an assay with the format shown in FIGURE 6 using a planar SPR substrate (i.e., comprising a conductive film without an overlying matrix). To obtain this data, a 50 nm thick Au film was first modified with 3-mercaptopropionic acid (MPA), thereby forming a carboxylate terminated self-assembled monolayer (SAM). The SPR profile obtained from this modified film alone is shown by the solid line trace in FIGURE 7A. Then,  $\gamma$ -chain-specific monoclonal goat anti-human IgG antibody [a-h-IgG ( $\gamma$ )] (the “first antibody” or “the primary antibody”) was coupled to the carboxylated monolayer via carbodiimide coupling to free amine moieties on the antibody. Incubation of the modified film with a 0.09 mg/mL solution of human IgG [h-IgG; 150 kD] (the “target antigen”) produced only a 0.04° shift in the plasmon angle. This is illustrated by the dotted line trace in FIGURE 7A. Indeed, the SPR profile in the presence of the antigen, h-IgG, is almost superimposed over the SPR profile obtained from the modified film alone because the plasmon angle shift is so small. Further exposure of this film to a 8.4 mg/mL solution of F<sub>c</sub> specific monoclonal goat anti-Human immunoglobulin G antibody [a-h-IgG(F<sub>c</sub>)] (the “second antibody” or the “secondary antibody”), results in only a small (0.06°) plasmon angle shift. This is illustrated by the dashed line trace in FIGURE 7A. However, when the secondary antibody is present as an electrostatic conjugate with 10-nm-diameter Au particle [a-h-IgG(F<sub>c</sub>)-Au], a 1.7° shift in plasmon angle is observed, accompanied by a 2% increase in minimum reflectance and a noticeable broadening of the SPR profile. This is illustrated by the dashed line trace in FIGURE 7B. This colloid-induced 1.7° shift is 28 times larger than that observed for the unamplified assay using the same planar substrate (i.e., the 0.06° as shown in the dashed line trace in FIGURE 7A). Thus, a significant increase in sensitivity is afforded through the use of protein-Au colloid conjugates in this biosensing embodiment. Biochemical specificity is also maximized under these conditions – surfaces modified with a-h-IgG( $\gamma$ ) show little or no reactivity with human serum (minus IgG), human immunoglobulin A, and [a-h-IgG(F<sub>c</sub>)-Au]. The a-h-IgG( $\gamma$ )-h-IgG modified surface is also highly specific, as exposure to a conjugate of 10 nm-diameter Au with goat anti-human immunoglobulin G1 (a-hIgG1-Au) leads to only a small (0.08°) plasmon shift. A more complete discussion of the materials and methods used in this immunoassay are provided in Example 2.



As mentioned previously, in preferred embodiments the assay is performed by measuring reflectance changes in the SPR substrate at a predetermined angle of incidence. The optimal angle is the one at which the largest change in reflectance is observed upon the occurrence of the biological event being detected. In the sandwich assay, this biological event is the formation of the primary antibody-antigen-secondary antibody "sandwich." To determine the optimal angle, a differential SPR profile (change in reflectance against the angle of incidence) is prepared by calculating the difference between the SPR profiles obtained for the secondary antibody and antigen steps. The peak of the differential profile occurs at the largest difference between the two spectra and thus represents the optimal angle for monitoring reflectance changes during that reaction.

FIGURE 8 represents a differential SPR profile for the data provided in FIGURE 7. For the case of the addition of a-h-IgG(F<sub>c</sub>), a maximum decrease in reflectance of only about 2% is obtained at an angle of incidence of 54.3° (dashed line trace in FIGURE 8). By contrast, for the addition of a-h-IgG(F<sub>c</sub>)-Au, a ~50% decrease in reflectance is observed at the same angle of incidence (solid line trace in FIGURE 8). Thus, the use of 10 nm Au-conjugated secondary antibody leads to a 25-fold increase in sensitivity relative to unconjugated secondary antibody.

FIGURE 9 shows reflectance time courses for the immobilization of both the unconjugated and Au-conjugated secondary antibodies. When the reaction is monitored at an angle smaller than the plasmon angle (53.4°, 50% reflectance), a change in reflectance of > 40% is observed in the case of the Au-conjugated secondary antibody (trace marked "Antibody: Au" in FIGURE 9), while immobilization of the unconjugated antibody to an identically prepared surface results in less than a <2% reflectance change (trace marked "Free Antibody" in FIGURE 9). This illustrates the sensitivity enhancement in assays that rely on the real-time monitoring of biospecific interactions. It should be noted that this enhancement is obtained despite the protein-Au conjugate being more than 6 orders of magnitude more dilute than the free antibody (17 nM vs 56 mM).

The utility of the particle enhancement methodology of the instant invention becomes most striking at low concentrations of antigen. FIGURE 10 illustrates the variation of the colloidal Au-induced plasmon angle shift as a function of h-IgG concentration. The h-IgG concentrations used are 3 mM (FIGURE 10A), 0.3 mM (FIGURE 10B), 3.0 nM (FIGURE 10C) and 6.7 pM (FIGURE 10D). In each figure, the

solid line represents the SPR profile for the a-h-IgG( $\gamma$ ) modified film; the dashed line represents the SPR profile of the a-h-IgG( $\gamma$ ) modified film in the presence of h-IgG only; the dotted line trace represents the a-h-IgG( $\gamma$ ) modified film in the presence of both h-IgG and a-h-IgG( $F_c$ )-Au. As expected, the observed plasmon shifts decrease as the solution antigen concentration is varied over nearly six decades (3.0  $\mu$ M to 6.7 pM). The lowest h-IgG antigen concentrations – 3.0 nM (FIGURE 10C) and 6.7 pM (FIGURE 10D) – induces SPR changes that are not detectable in the absence of a-h-IgG( $F_c$ )-Au. Despite these low antigen concentrations, significant shifts due to particle immobilization are still evident when the 10 nm Au-conjugated secondary antibody is used. Even at the lowest concentration of h-IgG investigated (6.7 pM=1.0 ng/ml), an easily detectable shift of 0.33° results (FIGURE 10D). The ease with which this shift may be resolved reveals that the actual detection limits for 10 nm Au conjugated secondary antibody are lower than even the picomolar range.

The immunosensing embodiments described above all use planar SPR substrates (i.e., Au films modified with a monolayer of a bifunctional organic linker to which the primary antibody becomes covalently bound). As discussed in the Background of the Invention, commercially available SPR assays typically use a Au film coated with an extended (e.g., 200 - 400 nm thick) carboxylated dextran matrix to concentrate capture molecules, such as primary antibodies. Molecules to be localized to the film surface (e.g., primary antibodies) are covalently bound by the dextran matrix, resulting in the formation of a three-dimensional array of molecules extending ~200 nm away from the surface. There are numerous drawbacks to using such a matrix, as outlined in the Background of the Invention. The methods of the instant invention dramatically surpass the sensitivity of such prior art matrices. For example, using 10 nm Au-conjugated secondary antibody on a planar SPR substrate leads to a 3,000 fold enhancement in detection limit relative to the same assay performed in dextran matrices using unconjugated secondary antibody.

In some embodiments of the invention, even further enhancements are obtained by using colloidal Au nanoparticles that are greater than 10 nm in diameter. For example, if the immunoassays described above are performed using 41 nm Au-conjugated secondary antibodies and a planar SPR substrate, then a 30-fold amplification in sensitivity is obtained over the same assay using 11 nm Au-conjugated secondary antibodies.

Compared to conventional SPR assays using dextran matrices, this represents a 100,000 fold increase in sensitivity. Indeed, using 41 nm Au-conjugated secondary antibodies and a planar SPR substrate, it is possible to detect h-IgG at a concentration as low as 10 pg/ml.

In some embodiments of the invention, conventional dextran-based matrices may  
5 be used as the substrates for colloidal Au-enhanced SPR sensing. However, depending on the matrix pore size, colloidal Au particles of the sizes used above may be excluded from the interior of the matrix by steric hindrance. A different methodology is required for such embodiments: colloidal Au nanoparticles small enough to enter the matrix are used and then, after their entry into the matrix, they are selectively enlarged by the addition of a  
10 metal plating solution, such as a solution of  $\text{Au}^{3+}$  and  $\text{NH}_2\text{OH}$ , or preferably a commercial Ag plating solution. In this way, the Au nanoparticles can be grown by the plating solution within the matrix to a size that significantly enhances the SPR response. For example, for the sandwich immunoassay described above, 1.8 nm colloidal Au can be conjugated to secondary antibodies. The resulting conjugate can diffuse into the matrix  
15 (within which primary antibodies are covalently bound), along with the target analyte to be detected. Following the creation of (primary antibody)–(target antigen)–(secondary antibody) complexes within the matrix, an Ag plating solution is passed over the film to enlarge the colloid size. Using commercial Ag plating solution, it is possible to selectively enlarge the conjugated Au nanoparticles, without nucleating new particles. In preferred  
20 embodiments, the Au film substrate upon which the dextran is overlaid is first pre-treated with a short chain alkane thiol, such as 6-mercaptohexanol, to prevent the Ag plating solution from plating Ag directly onto the Au film through holes in the dextran matrix. When this method is used to perform the h-IgG immunoassay described above, a 30-fold enhancement is obtained over the same assay performed with 41 nm Au-conjugated  
25 secondary antibody. A  $10^6$ -fold enhancement is obtained relative to the same dextran-based assay performed using unconjugated Au secondary antibody.

It will be appreciated that all of the aforementioned immunosensing embodiments can be adapted for the detection of any target analyte for which suitable primary and secondary antibodies are available. In addition, it will be understood that the methods  
30 described are applicable to any molecular recognition assay in which one of the participants in the molecular recognition event can be immobilized on a planar SPR substrate, and another participant can be conjugated to colloidal Au nanoparticles. For

example, a receptor-ligand interaction can be assayed by immobilizing a receptor on a planar SPR substrate, and then either conjugating the ligand directly to colloidal Au, or by using a colloidal Au-conjugated antibody that can bind to the ligand. Furthermore, the methods of the invention can be used to study desorption of Au-colloid tagged reagents from the Au film, rather than interaction-driven adsorption.

The methods describe herein provide two examples of SPR based assays based on molecular recognition: (1) an assay in which one of the molecules that participates in the recognition event is immobilized on a derivatized, planar SPR Au film substrate, and another of the molecules that participate in the recognition event is conjugated to colloidal Au of size ~10 – 150 nm; or (2) an assay in which one of the molecules that participates in the recognition event is immobilized within a dextran matrix overlaid onto a Au film, and another of the molecules is conjugated to colloidal Au of a diameter sufficiently small to permit the conjugated reagent to diffuse into the dextran matrix; following diffusion of the conjugate into the matrix, the Au nanoparticles are enlarged by the addition of Ag plating solution. Both strategies provide unique methods of signal amplification and the better method is best determined by evaluating some general criteria. Other criteria, in addition to that presented below, will be apparent to those of skill in the art in determining the best method for a particular purpose.

Most important is the size and nature of the capture molecule (e.g., “Ligand A” or the “primary antibody”) and analyte to be immobilized. Large molecules could be excluded from diffusing into the dextran; thus the most sensitive region – close to the surface – is unavailable. Likewise, if the analyte is large, diffusion to the immobilized receptor may be impossible. Dextran matrices are also impractical if a particular orientation of the capture agent is necessary for receptor binding, as is the case for DNA hybridization or membrane studies. Many protocols are known in the art to correctly orient DNA, bilayer membranes, or proteins onto a planar surface.

The concentration of the target molecule should also be considered. With respect to h-IgG, low concentrations (100 ng/ml-100 pg/ml) are well suited for the Au enhancement on a planar film with 11-nm diameter Au colloid; and lower concentrations require larger colloids. However, the latter species are more likely to denature (though not usually observed). Also, there is an increased possibility of multiple interactions between the protein-bound particle and the surface. In contrast, 1.8-nm diameter Au colloid

conjugates offer (in most cases) a 1:1 protein to colloid ratio. This should aid in quantification and, with optimized exposure time to the Ag plating solution, should afford detection at very low concentrations (<100 pg/ml). However, after Ag plating, further immunochemical manipulations are impossible. Finally, it should be noted that both  
5 surfaces are amenable to regeneration using standard techniques.

Greater changes in the SPR angle shift are expected for particles able to couple more efficiently to the surface plasmons in the Au film. Thus, one embodiment of the invention is directed to generating particles with tunable absorbance spectra for use as SPR tags. Absorbance of light by Au nanoparticles leads to excitation of particle-based  
10 surface plasmons, an effect that is size dependent. Thus, one simple means of tuning the absorbance spectrum for SPR tags is to use different sizes of Au nanoparticles. Two of the problems traditionally associated with larger colloidal Au nanoparticles (i.e., those with diameters greater than 35 nm) have been polydispersity and instability (relative to smaller particles). Since it is known that the stability of colloidal particles decreases with  
15 increasing size, it follows that part of the instability problem could be solved through improved monodispersity. Moreover, for applications in which the Au nanoparticles are *reagents*, it is essential to have "reagent-grade" (i.e., relatively pure) materials.

While it is easy to understand that larger changes in reflectivity are observed for larger particles (presumably due to both the scattering and greater changes in the dielectric  
20 associated with the binding of more Au metal per particle), significant changes were not expected for the very small molecular Au clusters. Although smaller particles give less dramatic shifts than are observed for larger Au tags, their smaller "footprint" allows a higher degree of labeling on the surface, and makes it easier to arrange for single particle binding events to correspond to single biological binding events. An added advantage of  
25 decreased particle tag size is improved diffusion of the tagged biomolecule.

Another example of the utility of colloidal Au reagents in biochemical SPR experiments involves binding and displacement of a colloidal Au-tagged protein. In an example of this embodiment of the invention, anti-biotin was covalently bound to a planar SPR substrate. Introduction of biotinylated colloidal Au (prepared by adsorption of  
30 biotinylated BSA to 10-nm Au) leads to a small change in reflectivity indicative of a low coverage of conjugate, which is in turn indicative of a small amount of active anti-biotin on the surface. When the antibody: antigen-Au complex is exposed to a high

concentration of biocytin, a water-soluble analogue of biotin that binds to anti-biotin, the colloidal Au tagged biotin is displaced, and the SPR reflectivity returns to its original position. These experiments show that binding of colloidal Au conjugates to SPR surfaces is reversible, and thus allows the use of SPR to detect binding of low MW species by  
5 ligand displacement.

Having shown that Au-particle amplification can lead to very large improvements in the sensitivity of SPR using standard IgG immunoassays as a model system, this technique has been applied to several other systems, e.g., to detection of biologically-important soluble factors in blood serum; for example, the cytokine interleukin-5 (IL-5).  
10 IL-5 is produced by T-lymphocytes and appears to be the main cytokine involved in the control of eosinophilia. Since eosinophils are important in allergy, IL-5 is thought to be of key importance in the development of allergic diseases (e.g., asthma). The pharmacological importance of IL-5 and other cytokines makes these molecules good targets for biosensing. The selectivity of IL-5: Au conjugate to protein A/anti-IL-5 on an  
15 Au film is shown in FIGURE 15. The observed angle shift was far greater for the specific interaction than for a nonspecific interaction (ST4: Au conjugate). There was a small amount ( $0.1^\circ$ ) of non-specific binding with ST4: Au. The specific interaction shifted the minimum  $1.6^\circ$ . (0.5% Blotto was used in these experiments to inhibit nonspecific binding). While this experiment illustrates both the sensitivity of Au-amplification and the  
20 selectivity of this assay, biological samples will contain free cytokines, not cytokine: Au conjugate. To detect IL-5 in such samples, a pseudo-competitive assay may be used. In this experiment, the protein A/anti-IL-5 coated Au film is exposed first to free IL-5 in the presence of a high concentration of human serum albumin, to mimic serum. After collection of the SPR curve, the surface is exposed to IL-5: Au conjugate. Due to the slow  
25 dissociation kinetics for anti-IL-5/IL-5 interaction, little if any IL-5 is displaced from the surface upon exposure to conjugate, but rather that IL-5: Au binds only to "open" antibody on the surface. Thus, the amount of angle shift resulting from exposure to conjugate is inversely proportional to the amount of analyte in the initial ("serum") sample.

In preferred embodiments of the invention, even further enhancements of the  
30 colloidal Au-conjugated SPR response are obtained by optimizing the coupling distance between the Au nanoparticles and the Au film. In some embodiments, an inorganic spacer, preferably  $\text{SiO}_2$  deposited through thermal evaporation, is placed over the surface

of a Au film to increase the distance between the colloidal Au and the Au film. In other embodiments, optimization of the coupling distance is achieved by overlaying the Au film with one or more polymer layers, preferably polystyrene sulfonate and/or polyallylamine hydrochloride built up through electrostatic interactions. In an especially preferred

5       embodiments, a 30-40 nm thick layer of SiO<sub>2</sub> is used in conjunction with 12 nm colloidal Au. FIGURE 11 illustrates the progressive enhancements in SPR response that occur when a Au film is coated with a 15 nm (FIGURE 11A), 24 nm (FIGURE 11B), and 33 nm (FIGURE 11C) thick layer of SiO<sub>2</sub> and then has 12 nm colloidal Au adsorbed thereon. In each figure, trace A is the SPR profile of the Au film without the SiO<sub>2</sub> layer or localized

10       Au colloid; trace B is the SPR profile of the Au film with the SiO<sub>2</sub> layer only; trace C is the SPR profile of the Au film with the SiO<sub>2</sub> layer and Au colloid attached. It is understood that the thickness of a spacer overlayer producing a maximum shift for a certain amount of immobilized colloid depends on (i) the thickness of the Au film; (ii) the composition of the film (different results would be obtained for Ag films, for example);

15       (iii) the excitation wavelength; (iii) the size of the colloidal Au particles; (iv) the composition of the colloid (different results would be obtained for colloidal Ag, for example); and (v) the surface coverage. In addition, it will be understood that there are many other materials that can be suitable spacers, including but not limited to, metal oxides, sulfides, nitrides, or any other material that contains metal ions in a positive

20       oxidation state.

For SiO<sub>2</sub> overlayers, a 30 nm thickness improves sensitivity 3-fold. Similar results have been observed for polymeric spacer layers composed of alternating cationic and anionic polymers. Not only does this development lead to improved detection limits, it also opens up all the attachment chemistries used on glass surfaces, and can improve film

25       stability.

The SiO<sub>2</sub> coating, while thin and certainly somewhat porous, also serves to protect the underlying metal from chemical attack. While reactivity is not a concern for Au films, oxidation can prevent the use of Ag metal for SPR. Ag films are known to have sharper angle-dependent reflectivity curves, and could be a better choice of substrate if not for

30       their rapid oxidation.

It is an important aspect of the present invention that the distance of the colloidal nanoparticle from the metal film can be essentially measured by the SPR detection.

Because of this property, it is not necessary that assays being conducted on the film surface require the presence or absence of the colloidal nanoparticle. Rather, according to the present invention, it is possible to conduct an assay whereby the presence of an analyte acts to increase or decrease the distance of the colloidal nanoparticle from the metal film surface.

Preferred embodiments of the invention use colloidal Au nanoparticles to enhance the SPR profile of metal SPR substrates. However, it is to be understood that the metal nanoparticles can be comprised of other materials with complex indices of refraction, including but not limited to Ag, Cu, Al, or alloys comprised of two or more of Au, Al, Ag, and Cu. In other embodiments, the metal nanoparticles comprise a core of Ag, Al, Au, or Cu (or an alloy of two or more of these metals) substantially covered by a shell of any metal, any oxide, any sulfide, any phosphide, or any organic or inorganic polymer. In addition, although preferred embodiments employ metal nanoparticles that are substantially spherical, it is to be understood that other shapes are also contemplated.

A wide range of wavelength "tunability" is possible for AuS core/Au shell particles, which have been described by the groups of Haus and Halas. See, e.g., Averitt *et al.*, Phys. Rev. Lett. 78:4217-4220 (1997). By varying the preparation conditions, it is possible to tune the position of the second  $\lambda_{\text{max}}$ , indicative of a control of the ratio of core to shell size. FIGURE 16 shows optical spectra for several batches of these particles. Particles having significant absorbance at 632 nm are particularly useful, as that is the laser wavelength most commonly employed in SPR work. Strong absorbance of light at the wavelength of the surface plasmon results in a high degree of film-nanoparticle coupling, which in turn leads to large SPR response and increased sensitivity.

Polydispersity in particle preparations leads to difficulties in interpreting SPR data, as amplification is a function of particle size. Synthesis of AuS/Au shell particles by methods analogous to those used for colloidal Au (i.e., rigorous cleanliness, ultrafiltered solvents, rapid reagent addition, rapid stirring and reflux) leads to marked improvement in monodispersity. Quantitative measurement of extinction coefficients are made on the resulting AuS/Au particles, both in solution and on surfaces. On surfaces, particle coverage is unambiguously established by AFM and FE-SEM. In solution, S and Au atomic absorption is carried out on a sample of the as-prepared sol in which all particles



have been removed by aggregation/centrifugation. This permits determination of whether 100% of the added Au was converted to dispersible particles. Subsequently, a combination of TEM image analysis and static light scattering is used to establish mean particle size and dispersity. These numbers can in turn be used to calculate a particle concentration in solution. For both sets of measurements, the observed data may be correlated to theory using Bohren's program for calculation of core-shell absorption and scattering.

To determine the optimal conditions for core/shell particles in ultrasensitive SPR applications, SPR spectra is collected at multiple wavelengths, and the results compared with expected behavior based on optical spectra for the particles. Of course at each wavelength, a different Au film thickness and different collection angle may be optimal; the relationships between these parameters are given by the Fresnel equations, and can be modeled very efficiently using available software.

#### 15 Ultrasensitive SPR detection of DNA hybridization.

In certain preferred embodiments, the colloidal Au enhancement methods of the instant invention are used to detect DNA hybridization. In one embodiment of the invention, a solution suspected of containing a target DNA sequence is treated with reagents that conjugate colloidal Au to nucleic acids within the solution. Following conjugation, the solution of nucleic acids is contacted with a planar SPR Au film substrate that has been modified with an oligonucleotide probe having sequence complementary to the target DNA sequence. If the target is present, it will hybridize to the immobilized probe, thereby bringing colloidal Au to the surface of the Au film. The resulting change in the SPR response of the film can be monitored to detect the presence of the target.

25 Methods for the attachment of nucleic acids to metal films are well known in the art. For example, amine modified nucleic acids can be attached to a 16-mercaptohexadecanoic acid-derivatized surface via 1-ethyl-3-(3-dimethylaminopropyl) carbodiimide/N-hydroxysulfosuccinimide crosslinking to carboxylate groups. Methods for DNA attachment to Au films are provided in Herne *et al.*, J. Am. Chem. Soc. 119: 8916-8920 (1997), incorporated herein by reference in its entirety.

30 In some preferred embodiments, a "sandwich assay"-type hybridization format is used for DNA detection; an example is illustrated schematically in FIGURE 12. In this

example, an oligonucleotide probe (S1) which has a sequence complementary to a first portion of the target DNA sequence (S2) is immobilized on the surface of a planar SPR substrate. The SPR substrate is then contacted with a solution suspected of containing the target DNA sequence (S2), and also with a colloidal Au-conjugated oligonucleotide (S3: Au) having a sequence complementary to a second portion of the target sequence. The sequences of S1 and S3: Au are designed such that in the presence of the target (S2), the sequences S1, S2 and S3: Au form a tripartite hybridization complex. In this way, colloidal Au is brought to the surface of the Au film only if the target sequence (S2) is present. The resulting changes in the SPR response of the film can be monitored in order to detect the presence of the target sequence.

The colloidal Au can be conjugated to the oligonucleotide (S3) by any of a number of methods known in the art. For example, thiol labeled DNA can be prepared, and the thiol group can serve to couple the DNA to Au as described in Mirkin *et al.*, Nature 382: 607-609 (1996), Elghanian *et al.*, Science 277: 1078-1081 (1997), Storhoff *et al.*, J. Am. Chem. Soc. 120: 1959-1964 (1998), Storhoff and Mirkin, Chem. Rev. 99: 1849-1862 (1999), and Mucic *et al.*, J. Am. Chem. Soc. 120: 12674-12675 (1998), each of which is incorporated herein by reference in its entirety. Alternatively, biotinylated DNA can be prepared, and then conjugated to streptavidin: Au conjugate. Example 3 provides a detailed protocol for the preparation of such conjugates. In some embodiments, the SPR substrate is treated with mercaptohexanol which helps the immobilized probe DNA to "stand up" by decreasing physisorption.

FIGURE 13 shows an example of an SPR profile obtained using the abovementioned assay format. In this example, the target (S2) is a 24-mer oligonucleotide. S1 and S3: Au are 12 mer probe oligonucleotides each of which is complementary to one half of S2. S1 has a 5' amine group through which it was immobilized to the Au film as described above. S3 has a 3' thiol group to which colloidal Au is attached. S1, S2, and S3 have the following sequences:

5' - H <sub>2</sub> N-C <sub>6</sub> H <sub>12</sub> - CGC ATT CAG GAT - 3'	S1
5' - TAC GAG TTG AGA ATC CTG AAT GCG - 3'	S2
5' - TCT CAA CTC GTA - C <sub>6</sub> H <sub>12</sub> -SH - 3'	S3

Trace A in FIGURE 13 shows the SPR response of the S1 conjugated Au film in the absence of the other reagents. Trace B shows that in the absence of S3: Au, the hybridization of S1 to S2 leads to only a very small angle displacement ( $0.1^\circ$ ) for the SPR reflectivity minimum. Trace C shows that when the S3: Au conjugate is added, there is a pronounced plasmon angle shift, which corresponds to an approximately 18-fold increase in SPR response compared to what was observed in the absence of S3: Au.

In certain preferred embodiments, the Au film is overlaid with a spacer in order to optimize the coupling distance between the Au film and the colloidal Au, as described above. The preferred spacer is a layer of  $\text{SiO}_2$ .

It will be appreciated that application of the Au-colloid SPR enhancement methodology need not be restricted to DNA detection assays with the probe configuration described above. There are many different assay formats known in the art for the detection of specific DNA sequences that rely on two central elements: (1) an immobilized probe (or probes) complementary in sequence to a portion of the target DNA sequence of interest; and (2) a detectable tag conjugated to a molecule that becomes associated, either directly or indirectly, with the immobilized probe. It will be appreciated that the methods of the instant invention can be readily adapted by one skilled in the art to enable SPR detection of target nucleic acid sequences in any assay format that relies on these two elements. Moreover, the same methodology can be applied to configurations in which the probes and/or target consist of other nucleic acids (e.g., RNA), nucleic acid analogs (e.g., peptide nucleic acids, etc.), or a combination thereof.

One of the unique features of SPR-based assays is that binding data can be acquired in real time to monitor the progress of the reaction. The inset to FIGURE 13 shows the kinetic plot of the second hybridization step (i.e., the probe: Au conjugate binding to surface-confined oligonucleotides) by monitoring the SPR reflectivity changes at a fixed incident angle,  $53.2^\circ$ , as a function of time. As expected, the signal changes dramatically in the first 5 minutes, with the hybridization process being nearly complete after 60 minutes.

The changes in the SPR response of the Au film can be reversed via DNA "melting" (i.e., dehybridization by heating the substrate), or by DNA digestion of the tripartite complex at a site that releases the Au nanoparticles. Again, the melting or DNA digestion can be monitored in real time to obtain kinetic data. In the case of DNA melting

studies, exact changes in temperature at a metal film induced by pulsed or continuous laser irradiation can be exactly calculated. Detection of single nucleotide polymorphisms (SNPs), for which hybridization/dehybridization thermodynamics and kinetics are highly temperature sensitive, can be achieved by monitoring the SPR response of the Au film in response to precise laser-induced temperature variations on the surface of the Au film. In the case of DNA digestion, cleavage of the surface confined oligonucleotide/probe: Au complex – either in a single or double stranded region – will be observed as a shift in the plasmon angle as the bound colloid gold is released.

As discussed above, the methods of the instant invention using scanning SPR allow the detection of less than  $3 \times 10^6$  particles/cm<sup>2</sup> for 45 nm diameter Au-colloid nanoparticles. If each particle is conjugated to a nucleic acid probe as described above, it is possible to detect  $3 \times 10^6$  target nucleic acid copies/cm<sup>2</sup>. DNA hybridization assays are commonly performed in a microarray format using reagent spots of around 50  $\mu$ m in diameter, as described in Bowtell, Nat. Genet. Suppl. 21:20-24 (1999), incorporated herein by reference in its entirety. Assuming a 50  $\mu$ m spot size, this means that the Au-colloid SPR enhancement methods herein provided are capable of detecting as little as 60 copies of a target nucleic acid. Even lower levels can be expected using larger Au colloid nanoparticles >45 nm in diameter. This level of sensitivity is unprecedented in the art. The methods herein provide new opportunities for PCR-free hybridization biosensors and for DNA diagnostics in general.

#### Imaging SPR and Microarray Assays.

The technique of imaging SPR is used in some embodiments to monitor analyte binding to a microarray, such as a microarray of DNA probes on a Au film-based SPR substrate. In conventional scanning SPR, SPR reflectivity is measured as the angle of incidence is varied through the angular range within which SPR occurs. Hence, at each angle of incidence, a single measurement of the SPR reflectivity of the entire SPR substrate is obtained. By contrast, in imaging SPR embodiments, a fixed angle of incidence is used, and the light that undergoes total internal reflection is imaged, preferably onto the surface of a charge coupled device (CCD). The resulting image spatially depicts SPR reflectivity variations. The changes in SPR reflectivity result from

localized changes in the refractive index near the surface of the SPR substrate; these latter changes in turn result from the adsorption or desorption of material at the surface of the SPR substrate. Hence, the reflectance image can reveal sites on the SPR substrate where such binding and desorption events have taken place.

5           In preferred embodiments, the colloidal-Au reagents described above are used as contrast agents for imaging SPR. The image is preferably captured at the angle at which the greatest increase in reflectivity is observed upon binding of colloidal-Au tagged reagents to the Au film. In the resulting image, regions of highest intensity represent areas of the Au film that have undergone the largest increases in reflectivity, and hence have  
10       bound the largest amounts of colloidal Au. As described above, the angles of maximum reflectivity change (the maximum increase and the maximum decrease in reflectivity) can be readily determined by subtracting the SPR profile of the "bare" Au film (i.e., without bound colloid) from the SPR profile obtained when colloidal Au binds to the Au film.

          In preferred embodiments, the CCD camera is configured such that the "bare" Au  
15       film appears black in the reflectance image. In this way, any changes in reflectance can be readily observed above the "background" reflectance of the Au film.

          In preferred embodiments, the SPR substrate is imaged at the angle of incidence at which the maximum increase in reflectance is observed upon colloidal-Au adsorption. However, it will be appreciated that the substrate can also be imaged at the angle of  
20       incidence at which the greatest decrease in reflectance is observed upon adsorption of colloidal Au.

          Because imaging SPR simultaneously gives reflectance data for multiple discrete regions of the Au film, this technique enables SPR-based microarray assays to be performed. In these embodiments, reagents – such as antibodies, DNA probes, etc. – are  
25       localized to specific discrete regions of the Au film. In preferred embodiments, a different reagent is immobilized to each discrete region. Methods for the arraying of biomolecules in this manner on solid supports are well known in the art. A fluid suspected of containing targets of interest is then contacted with the Au film, along with colloidal-Au conjugated reagents as described above. The Au film is then imaged using the imaging SPR  
30       apparatus. The normalized reflectance intensity at each region on the Au film reveals the amount of target that has bound thereto; the position of the reflectance signal reveals the identity of the target. In this way, it is possible simultaneously to quantify multiple

targets. Moreover, it is also possible using the methods of the invention to obtain kinetic data simultaneously for multiple targets (e.g., for DNA polymorphisms).

In some embodiments of the invention, assays are performed using mixtures of more than one size of colloidal-Au nanoparticles. Because the angle of maximum  
5 reflectance change varies with nanoparticle size, in such embodiments it is necessary to image the SPR substrate at more than one angle of incidence. For example, using a 50 nm thick Au film, a large reflectance change is observed at 70° when 10 nm colloidal Au becomes localized to the Au film, but no change is observed at this angle when 35 nm Au colloid becomes localized to the film. However, if the angle of incidence is raised to 73°,  
10 then a large reflectance increase is observed for 35 nm Au-colloid, but not for 10 nm Au-colloid. Thus, measurement at both angles may be used to determine the amount of each particle type present.

In preferred embodiments, an imaging SPR instrument is used in which the SPR substrate is oriented horizontally. This can be done by placing the prism base facing  
15 upright in the horizontal plane. The SPR substrate can then be placed on top of the prism base, and optically coupled to the prism using, for example, a drop of immersion oil. In strongly preferred embodiments, the prism is mounted on a rotational stage in order to accommodate adjustment in the incident angle.

The horizontal prism geometry provided by the instant invention allows for two  
20 significant improvements over SPR instruments used in the art. First, positioning the SPR substrate parallel to the laser table (i.e., in a horizontal, face-up orientation) allows the rapid and parallel introduction of solutions and reagents to the sample surface. Indeed, very simple experiments may be performed with all solution chemistries contained in a droplet atop the sample. Liquid reagents may also be introduced robotically in this  
25 geometry, as opposed to prior art vertical sample positioning where solution must be flowed to the substrate. Secondly, the absence of a complicated flow cell for the introduction of liquids requires only that the sample be placed atop the prism in order to acquire an image. Substrates may be rapidly interrogated in a serial fashion in this arrangement, much in the same way 96-well plates are introduced to plate readers.  
30 Accordingly, the possibility for robotic introduction of substrates is greater in this horizontal geometry than in a prior art vertical sample orientation.

FIGURE 14 illustrates in front elevation perspective a preferred embodiment of the imaging SPR configuration outlined above. The instrument is mounted on an optical bench 13. The excitation source 1 is preferably a laser, most preferably either a 1 mW HeNe laser (632.8 nm, 500:1 polarization) or a  $\text{Ar}^+/\text{Kr}^+$  laser that permits excitation at multiple wavelengths. Laser light is passed through a neutral density filter 2, and then through a linear polarizer 3 to further increase the polarization extinction. Polarization is parallel with respect to the horizontal plane and is therefore *p* polarized at the horizontally oriented prism/sample assembly 8. Two mirrors 4 and 5 then steer the beam upwards, preferably at a  $20^\circ$  angle, from the surface of optical bench 13 into a spatial filter 6. Spatial filter 6 expands the beam, at which point the center of the beam is collimated by a plano-convex lens 7. Spatial filter 6 preferably comprises a 60X microscope objective with a  $5\text{ }\mu\text{m}$  pinhole, and preferably expands the beam to  $\sim 4.5$  inches in diameter. Plano-convex lens 7 preferably collimates the expanded beam to 3-inches in diameter. It is important to note that this dramatic beam expansion allows illumination of the sample with a wave front that has only a very slight spatial intensity fluctuation. This avoids potential background subtraction ambiguities in the acquired images.

Collimated light leaves lens 7 and enters the prism/sample assembly 8. The  $20^\circ$  upward beam angle provides the  $70^\circ$  angle of incidence at the prism/sample assembly 8 that is optimal for high contrast SPR imaging of thin Au films. In preferred embodiments, the prism/sample assembly comprises a  $70^\circ - 70^\circ - 40^\circ$  prism positioned such that its base is parallel to and facing away from the optical table 13. An SPR substrate, preferably comprising a 50-nm-thick Au film evaporated onto a microscope slide, is then optically matched to the prism base with a small drop of immersion oil. Coarse positioning of the sample holder is accomplished by sliding the prism/sample assembly 8 on a vertically mounted rail, while fine pressure adjustments are made with the micrometer-actuated translation stage. Attenuated total internal reflection of the expanded beam occurs, resulting in passage of the beam downwards to the collection leg of the apparatus. At this obtuse imaging angle, the reflected beam is compressed about one dimension as indicated in FIGURE 14. This is corrected by re-expanding and collimating the image with a pair of hemicylindrical plano-convex lenses 10 and 11. The beam is then refocused onto and collected by the charge coupled device (CCD) camera 12.

Because the beam is deflected upwards by mirrors 4 and 5 from the surface optical bench 13, optical elements 5 through 12 in FIGURE 14 are preferably mounted on a high-stability rail system to provide a rigid structure. In preferred embodiments, mirrors 4 and 5 and the rail system can be adjusted to vary the angle of incidence and collection over the entire useful SPR range (i.e., from about 45° to about 80°).

Imaging SPR instruments are generally considered to be less sensitive than scanning SPR instruments. However, using the imaging SPR instrument and the Au-colloid (12 nm) enhancement methods of the instant invention, has allowed the reliable detection of approximately  $8 \times 10^7$  oligonucleotides/cm<sup>2</sup> in multispot arrays, with a dynamic range of greater than five orders of magnitude. This result was obtained without making any attempt to optimize hybridization efficiency, and represents a two to four order of magnitude improvement in sensitivity as compared to values provided in the literature for scanning SPR instruments without Au-colloid enhancement. The unoptimized sensitivity of microarray scanning SPR with Au colloid enhancement is at least comparable to that of conventional fluorophore-based methods for the detection of target DNA sequences in microarrays. However, use of the instruments, methods and reagents of the present invention will provide sensitivities that surpass fluorophore-based systems. Optimizing the improvements in Au colloid selection (e.g., size, shape, composition, etc.) and hybridization protocols (e.g., probe selection, annealing conditions, etc.) will be a routine task for those skilled in the art.

There have been significant improvements in the geometries for and approaches to creation of surface plasmons. Embodiments of the present invention directed to the implementation of some of these embodiments are described below.

Simple SPR interferometers have been described in the literature. In the work of Kabashin and Nikitin, for example, a beam is split prior to Kretschmann-geometry surface plasmon excitation and then recombined with the reflected light. Kabashin and Nikitin, Opt. Comm. 150: 5-8 (1998). The resulting interference pattern was imaged using a CCD. At the resonant angle of 43.7°, the minimum change in refractive index that could be detected was  $\Delta n = 4 \times 10^{-8}$ , two orders of magnitude lower than can be detected by measurement of shifts in angle. In one embodiment of the present invention, the measurements can be performed using 12-nm diameter colloidal Au amplification, so that coverages of Au too low to be detected by shifts in angle (but clearly present based on



AFM data) can be detected interferometrically. No detectable scattering is expected with such a low coverage of small nanoparticles.

In another embodiment of the present invention, the sensitivity of colloidal Au-amplified SPR may be improved by use of a "poor man's photonic crystal." Photonic crystals are materials that are completely opaque at certain wavelengths and completely transmissive at others. It has been shown that surface plasmons enhance optical transmission through subwavelength hole arrays in thin Ag films. Two anomalous effects have been observed: First, there are well-defined transmission minima and maxima, as would be expected for a photonic band-gap material. Second, the transmission through the holes is a thousand times greater than that predicted by standard aperture theory. This indicates that light flux at the holes is enhanced via coupling to surface plasmons. The present invention may take advantage of the enhanced coupling between the hole and a metal nanoparticle inside the hole. To do so, thin Ag films on glass with arrays of holes (of 100 nm in diameter) may be prepared similar to those described in the literature. The Ag surface may then be coated with an organothiol SAM to allow the glass beneath the hole to be selectively derivatized with capture antibody. A sandwich immunoassay may then be performed, with the secondary antibody tagged with a colloidal Au particle. Introduction of a colloidal Au particle then leads to a large change in the optical properties of the array of holes (e.g., reflectivity, transmittance). Even greater changes may be seen upon electroless growth of the particle to nearly fill the hole. Note that, since the film has been coated with an organoethiol SAM, metal will grow only on the particle.

In another embodiment of the present invention it is possible to simultaneously measure colloidal Au-SPR scattering over  $2\pi$  and reflectivity as a function of angle. A CCD is mounted on a rotation stage, and can move with the hemispherical prism, allowing the scattered light to be measured at all angles. As a result, there will be an entire scattering image for each reflectivity data point. Three attributes of the data are important. First, because the photodiode collects both scattered and reflected light, measurement of the scattered intensity reaching the CCD at a given angle of incidence allows the scattered and reflected light to be distinguished. This is an essential prerequisite to understanding SPR reflectivity at surfaces with immobilized large particles, which exhibit both scattering and reflectivity components. Second, the scattering images themselves are used to determine the size (or sizes) of colloidal Au nanoparticles bound to the surface as well as

to quantitate the number of particles bound. Third, there is an angular dependence and spatial distribution to the scattering. Both particle size and laser excitation angle profoundly impact scattering intensity.

5    Wet-chemistry synthesis of Au films.

          The need for specific thicknesses of evaporated Au presents a significant barrier to high-throughput SPR substrate generation. To address this problem, the present invention provides a rapid wet-chemical approach to obtain thin Au films. The approach uses a “seeding” mechanism. In preferred embodiments, a seeded film is prepared by the  
10   selective reduction of  $\text{Au}^{3+}$  ions from aqueous solution onto self-assembled monolayers of pre-formed colloidal Au particles. A detailed protocol for the wet chemical “seeding” of thin Au films is provided in Example 4.

PDMS microwell Arrays.

15           In order to quickly address multiple chemistries upon the same surface, a method is needed to physically separate each unique chemical interaction, enabling individual interrogation of each. One embodiment of the invention is directed to the fabrication and implementation of a polymeric, uniformly distributed, microwell array. The array of wells is biocompatible, extremely flexible, has very low chemical reactivity, can be attached to  
20   any substrate without use of adhesives, and is fabricated from inexpensive, readily available materials. These characteristics make the array an extremely flexible tool in implementing and analyzing arrayed chemistries, making it possible to carry out the simultaneous analysis of multiple surface chemistries by surface plasmon resonance (SPR). Such microwell array is also useful for analysis by ultraviolet-visible spectroscopy  
25   (UV-vis), surface enhanced Raman scattering, (SERS), and other surface-sensitive analytical techniques.

          Recent years have seen a marked increase in the use of arrays as a tool in chemistry. The rapidly increasing use of combinatorial chemistry and its application in high throughput screening account for the majority of array usage in chemistry.  
30   Combinatorial chemistry is utilized in chemical areas as diverse as drug and inorganic compound discovery and novel material synthesis. Arrays have also been increasingly used as sensors to perform analysis of distinct compounds in a chemical mixture, with

each individual sensor used to detect a unique compound. Alternatively, the individual sensors combine with the others in the sensor array to form a library of the ingredients in the addressed sample. Capillary electrophoresis columns arrayed on microchips is an example of an array adapted to an analytical technique.

5 Polydimethylsiloxane (PDMS) is a commercially available, inexpensive polymer possessing desirable properties for microwell arrays. The biocompatibility of PDMS makes it ideal for medical uses such as implants, artificial joints, contact lenses, and vascular and skin grafts. Industrial applications include electronics coatings and insulation, anti-foaming agents, media in carbon paste electrodes, micromachining, and  
10 microfabrication by microcontact printing (pCP) and micromolding in capillaries (MIMIC).

Fabrication of the PDMS microwell array of the present invention begins with the cutting of a section of electronic breadboard with a square pattern of 0.046-inch diameter holes spaced 0.092 inches on center. The PDMS prepolymer is then poured over the  
15 breadboard mold, and the prepolymer allowed to cure in a plastic petri dish. The PDMS-breadboard composite is then removed from the petri dish, and the components separated by hand. One of the potential problems with reproducing an array of this scale is that some of the posts become separated from the rest of the array. To prevent this, a light coating of release agent (e.g., Dow Corning 230 fluid) may be used on the  
20 breadboard mold. In addition, a thin layer of polymer may cure on the backside of the mold is easily shaved off with a razor blade. The PDMS "post array" cast is then used as a mold. Again, the mold is laid down in a petri dish (posts down) and PDMS is poured over it. Weight is placed on the mold to ensure proper contact of the post-tops with the petri dish surface. Again the prepolymer is cured. The PDMS "sandwich" is removed from the  
25 petri dish and separated. The new microwell array is then sonicated in soapy water followed by methanol for ten minutes each. FIGURE 17 shows the results of each molding step.

Adhesion tests were conducted on glass, doped silicon, polycarbonate, and evaporated gold on glass. The well arrays were attached to the clean substrates by  
30 pressing them to the surface by hand and allowing electrostatic adhesion to take place. Designated wells were then filled with a 0.01 M aqueous solution of bromocresol blue with a pipette. Adhesion stability was recorded at 10, 20, 60, and 720 minute intervals.

Even after 720 minutes of being attached to a given surface, no evidence of bromocresol blue leakage was observed on any of the substrates (FIGURE 18).

The well array masters show a remarkable integrity, as several of the post masters have been used many times to replicate well arrays with seemingly no increase in structural defects. Post masters have been replicated from several different sizes and patterns, with equal success and minimization of defects. The hole sizes may range from 0.001 inches to 0.5 inches in diameter, preferably from 0.025 inches to 0.1 inches, with a density of holes up to 400 per square inch. Well arrays can be layered on top of one another and used to form post masters with longer posts from which arrays with deeper wells can subsequently be produced. Pigments may also be introduced into the elastomer, before curing, to produce colored well arrays. The use of colored arrays cuts down on stray and reflected light and therefore may be more useful in analyses where the light source is irradiated through the individual wells.

The PDMS well substrates of the present invention serve as an easily fabricated and implemented method of physically separating individual chemistries on a substrate. Each of these wells can be individually addressed and the surface chemical interactions analyzed without cross-contamination. Accordingly, these arrays can be readily adapted to virtually any surface analytical technique.

#### Reduction of background signal.

The main source of noise in SPR measurements is background signal, i.e. non-specific binding of colloidal Au. One approach to further improve the quality of the colloidal reagents includes coating Au nanoparticles with SAMs formed from mixtures of  $\text{HS}(\text{CH}_2)_{15}\text{CO}_2\text{H}$  (10%) and  $\text{HS}(\text{CH}_2)_{10}\text{CH}_2\text{OH}$  (90%), the same composition of thiols used to coat substrates. The carboxylates on the particles will stick out by a number of carbons and therefore can easily be activated by EDC, but the large preponderance of alcohol groups on the surface will preclude non-specific binding. Also, by appropriate dilution of carboxylate, it is possible to control the number of available biomolecule attachment sites. In addition, to circumvent the possibility that the quality of biomolecule:colloidal Au conjugates change over time, the biomolecule:particle probes may be lyophilized.

Other means to reduce nonspecific binding, particularly in DNA hybridization experiments, include: controlling the temperature, adding noncomplementary sequences,

adjusting salt concentration, and reducing the solution concentration of DNA: Au conjugates during hybridization to surface oligos. To further decrease nonspecificity, longer linkers between DNA and the surface, both on colloidal Au particles and on the Au films may be used. Additionally, polyethylene glycol moieties can be covalently attached to carboxyl-terminated SAMs.

#### Increasing sensitivity by secondary amplification.

Increasing the magnitude of an Au nanoparticle-mediated change in reflectivity may be accomplished by directly amplifying the signal. This may be done by increasing the size of a colloidal Au nanoparticle that is brought in proximity to the SPR film via a binding reaction. Several different approaches to growth of immobilized colloidal Au nanoparticles, using both  $\text{Au}^{3+}$  and  $\text{Ag}^+$  (and appropriate reducing agents) have been demonstrated.

An alternative approach to direct amplification is to use a particle binding cascade, in which binding of a single particle triggers subsequent particle binding via specific nucleic acid (e.g., DNA) interactions. In one example, a colloidal Au “detection particle” (DP) is coated both with a monoclonal antibody that recognizes an antigen of interest and with a 30-base single-stranded DNA oligonucleotide (A). A first amplification particle (AP-1) comprising gold colloid coated with two single-stranded oligonucleotides (A' and B') is also prepared (e.g., by adding a mixture of biotinylated oligos to streptavidin: Au), where A' is totally complementary to the oligonucleotide on the detection particle, while B' is totally non-complementary. Binding of the antigen to a capture antibody leads to binding of DP. Subsequent introduction of AP-1 into the solution will result in binding of multiple AP-1 particles to the DP. A second amplification particle (AP-2), coated with a single-stranded oligonucleotide (B) complementary to B', may then be introduced which will result in binding of multiple AP-2 particles to the AP-1 particles. Indeed, this cascade scheme may be expanded to include additional amplification particles.

It is important to note that the non-linear response of reflectivity and scattering vs. particle size means that the amplification is non-linear as well: three particles bound in close proximity so as to behave optically as a single large particle will yield changes far greater than those observed by binding of three isolated small particles. Moreover, while it is possible to induce an entire network of particles to bind to a single bound particle,

such a network must necessarily have existed prior to binding to DP, as the DP cannot by itself induce networking. Since it is essential that there be no non-specific binding of DP, AP-1, or AP-2, an approach in which the cascade of nanoparticles is sequentially constructed is preferred to the task of eliminating non-specific binding of an aggregate.

5           An alternate cascade scheme may be used that does not require sequential addition of the amplification particles. This may be accomplished by designing the oligonucleotides attached to the amplification particles so that they are not complementary to each other, but are complementary to another single stranded segment of nucleic acid (e.g., DNA). This complementary oligonucleotide can be introduced into solution to  
10   activate the cascade that results in the binding of the amplification particles. For example, AP-1 may be coated with single stranded oligonucleotides B and C that are not complementary to each other or to A (which is coated on the DP). As described above, binding of the antigen to a capture antibody will result in binding of DP. However, AP-1 present in the solution will not bind to DP until single stranded oligonucleotide A'B'  
15   (complementary to oligos A and B) is introduced. Accordingly, AP-2 (which may also be present in the solution), coated with single-stranded oligonucleotide D, will not bind to AP-1 until oligonucleotide C'D' (complementary to oligos C and D) is introduced. As above, this cascade scheme may be expanded to include additional amplification particles. The advantage of this alternative scheme is that the amplification particles need not be  
20   added sequentially, but may be present in the solution from the start.

#### High-throughput screening of combinatorial libraries.

In one embodiment of the invention, particle-enhanced SPR is used in high throughput assays for libraries of small molecules. The combinatorial chemistry paradigm  
25   of drug discovery has created a situation where the design of functional assays is now rate-limiting, and few, if any, generally applicable solutions have been offered. The simplicity of SPR and its ability to be used in imaging mode make it an excellent choice.

High throughput applications require higher site density for SPR measurements. PDMS microwell arrays, with a "beaker" density of > 100 per sq. inch, provide such  
30   higher density of sites. While repetitive pipetting of such small volumes may be inconvenient (or impossible) to perform manually, it may be accomplished by use of an arrayer robot. The approach involves using the robot's eight dispensing pins to deposit

small spots of  $\text{HS}(\text{CH}_2)_{11}\text{CO}_2\text{H}$ . This molecule forms SAMs at those discrete locations on the substrate (i.e., where the dispensing pins came into close proximity). The remainder of the substrate is then filled in with  $\text{HS}(\text{CH}_2)_{15}\text{CH}_3$ , creating a hydrophobic environment around each (hydrophilic) spot. When the arrayer robot then dispenses an aqueous solution, it forms droplets over the hydrophilic patches, which provide the boundaries necessary to work at high site densities. An alternative solution is to use the robot's dispensing pins to mold a shape similar to them (but a bit larger) that can be filled with solvent.

10 Example 1.

Preparation of Evaporated Au Films and Au Colloid.

The following materials and methods were used to obtain the data presented in FIGURES 1-5.

Au colloid of  $<12$  nm diameter was prepared by citrate reduction of  $\text{HAuCl}_4 \cdot 3\text{H}_2\text{O}$  as described in Grabar *et al.*, J. Anal. Chem. 67: 735-743 (1995) and Grabar *et al.*, J. Am. Chem. Soc. 118:1148-1153 (1996), each of which are incorporated by reference herein in their entirety.

Au colloid of  $> 12$  nm diameter was prepared by a modified "seed colloid" technique. 12 nm colloid (major axis  $12 \text{ nm} \pm 2 \text{ nm}$  and minor axis  $11 \text{ nm} \pm 1 \text{ nm}$  from 758 particles sized) in an amount of 1 mL was used as the starting material, with 100 mL, 0.01 %  $\text{HAuCl}_4$  and 500 mL of 38.8 mM citrate solution. The resulting sample as analyzed by transmission electron microscopy (TEM) showed a major axis of  $45 \text{ nm} \pm 5 \text{ nm}$  and a minor axis of  $37 \text{ nm} \pm 4 \text{ nm}$  from 274 particles sampled. A second batch of large colloid produced using 100 mL of 0.02%  $\text{HAuCl}_4$  and 1.0 mL of 38.8 mM citrate solution showed a major axis of  $59 \text{ nm} \pm 14 \text{ nm}$  and a minor axis of  $52 \text{ nm} \pm 11 \text{ nm}$  from 424 particles. Similar protocols produced batches of particles of the following dimensions:  $30 \text{ nm} \pm 3 \text{ nm}$  (major axis) x  $25 \text{ nm} \pm 2 \text{ nm}$  (minor axis) from 373 particles sized and  $35 \text{ nm} \pm 3 \text{ nm}$  (major axis) x  $30 \text{ nm} \pm 3 \text{ nm}$  (minor axis) from 112 particles sized. These preparations used 100 mL of 0.01%  $\text{HAuCl}_4$  and 500 mL of 38.8 mM citrate solution with 3 mL and 2 mL of 12 nm diameter colloidal "seed" added, respectively. Average particle diameter and standard deviations were determined by particle size analysis of TEM Images using NIH Image: v.1.62 software.

Thin (47-50 nm) Au films were prepared by thermal evaporation of Au shot (99.99%, Johnson Mathey) from a resistively heated molybdenum boat (Kurt J. Lesker) in a diffusion-pumped Edwards Auto 306 thin-film fabrication system. Evaporation substrates were 1 inch x 1 inch x 0.02 inch, pieces of polished SF11 glass ( $n = 1.78$ , Schott Glass Technologies) that had been exposed to a 10% (v/v) (3mercaptopropyl)-trimethoxysilane/CH<sub>3</sub>OH solution for 30 minutes in order to increase the adhesion of Au to the glass. Au was deposited at a pressure of  $1 \times 10^{-6}$  mbar at 0.5 nm/s with constant sample rotation to ensure uniform deposition. Following evaporation, the films were annealed in a home-built oven at 300 °C for 5-10 minutes under a constant flow of argon to decrease the surface roughness of the evaporated layer.

Annealed Au films were modified with alkanethiols (2-mercaptoethylamine (MEA) or 3-mercaptopropionic acid (MPA)) from 10 mM ethanolic solutions for a period of 30 min. Longer immersion times did not noticeably improve the efficiency or density of subsequent derivitization steps. Immobilization of colloidal Au onto amine modified (MEA coated) surfaces was performed from undiluted aqueous solutions at room temperature. Amine-modified surfaces induce the strong adsorption of colloidal Au particles by virtue of the availability of an electron lone pair on the amine nitrogen, as well as ionic interactions with the negatively charged particles.

SPR data was obtained using a scanning SPR instrument. Excitation of the surface plasmon is accomplished using the Kretschmann geometry where a 1 inch diameter hemispherical prism (SF11 glass, Esco Products) is index matched (Cargille immersion oil,  $n = 1.78$ ) to a SF11 substrate onto which Au had been previously evaporated as described above. This assembly is then affixed to a home-built flow cell (volume ~100 mL) with the Au film exposed to solution. The SPR excitation source is a cylindrical 5 mW, 500:1 polarization extinction HeNe laser (632.8 nm, Melles Griot) which is further polarized by a 500:1 visible-optimized linear polarizer (Newport 10LP-VIS). An optical chopper (Stanford Research Systems) is used to modulate the optical signal at a frequency of 2 kHz, which was then correlated with detection via a lock-in amplifier (Stanford Research Systems, SR530). The beam is focused by a 100-mm focal length (f1) plano-convex (PCX) lens and recollimated by a 25-mm f1 PCX lens, thereby reducing the beam size to  $0.4\text{mm} \pm 0.1\text{ mm}$  in diameter. A hemispherical lens is then used to focus the beam



such that it is recollimated by the hemispherical prism-sample assembly. The reflected beam is then passed through an iris and focused onto a silicon photodiode detector (Thor Labs), the signal from which is then measured with the lock-in amplifier that is in-phase with the excitation source. Angular positioning of the sample is accomplished with a

5 home-built  $\theta$ 2 $\theta$  stage consisting of two high-resolution (0.001°) servo-drive rotation stages (Newport, RTM80CC and RTM160CC annular rotary stages) that are mounted together such that their axes of rotation are collinear. The prism/sample/ flow cell assembly is then mounted on the  $\theta$ 2 $\theta$  stage such that the center of the Au/glass sample is at the axis of rotation. Stage rotation and data collection are controlled through a

10 computer interface that was developed using the LabVIEW programming language (version 4.01, National Instruments). A typical SPR scan was run at either 0.1 or 0.01° resolution, a stage rotation rate of 0.5° s<sup>-1</sup>, and a lock-in time constant of 0.3 s.

Particle densities were determined using Tapping mode atomic force microscopy (TM-AFM) images acquired using a Digital Instruments Nanoscope IIIA operated in

15 tapping mode with an acquisition frequency of 1.5 Hz and line density of 512. Standard 200 nm etched silicon probes were used for the purposes of coverage determination. At least four images were obtained from two distinct regions of each sample. Two 5  $\mu$ m x 5  $\mu$ m images were taken ~0.5 mm apart to confirm that the surface coverage was homogeneous. At each position, 1  $\mu$ m x 1  $\mu$ m scans were captured in order to obtain

20 higher resolution images. Particle counting was done manually from captured images. Reported numbers are average coverage values obtained from 2 to 3 images.

In all experiments, care was taken to ensure that the identical region of a particular sample was interrogated with both SPR and TM-AFM. Accordingly, a box was scratched around the area illuminated during the SPR experiment. The surface coverage within that

25 area was then measured via AFM, thereby alleviating any errors due to uneven surface derivatization over large length scales. It is important to note that the solution agitation is an important step in obtaining particle-diameter-independent coverage values. At short exposure times (< 1 hour) and identical solution particle concentrations, approximately equal particle surface concentrations may be obtained independent of colloid diameter.

30 This removes the diffusion dependence of surface attachment and leaves the sticking

probability (which is only slightly influenced by particle diameter) as the determining factor in the resultant particle number density.

Example 2.

5    Sandwich Immunoassays.

The following materials and methods were used to obtain the data presented in FIGURES 6-10.

Au film and Au colloid were prepared as described above. Human IgG (h-IgG),  $\gamma$ -chain-specific monoclonal goat anti-human IgG antibody [a-h-IgG ( $\gamma$ )] and  $F_c$  specific  
10    monoclonal goat anti-Human immunoglobulin G antibody [a-h-IgG( $F_c$ )] were obtained from Sigma Immunochemicals.

Protein-Au conjugates were synthesized by the addition of a-h-IgG ( $F_c$ ) to 5 mL of pH-adjusted colloid followed by incubation on ice with periodic gentle mixing for 1 hour. The conjugate was then divided into 1 mL fractions in 1.5 mL, micro-centrifuge tubes and  
15    centrifuged at 12,500g for 45 minutes (Heraeus picoBiofuge). The clear to pink supernatant was removed and the soft pellet resuspended to an optical density of  $\sim 3$  into  $H_2O$  or 40 mM phosphate buffer (pH 7.0). Conjugates can be stored between 2 and 8 °C for several days without loss of activity.

A flocculation profile was constructed for a-h-IgG ( $F_c$ )-Au colloid conjugates to  
20    determine the amount of protein that was necessary to coat the exterior of the Au particle, and hence inhibit colloid aggregation. Solutions were prepared from 0.75 mg/mL stock solution aliquots (0-72  $\mu$ g) of a-h-IgG ( $F_c$ ) and were added in 6  $\mu$ g increments to cuvettes containing 1.0 mL of 10 nm diameter colloid solution adjusted to pH 8.0 (EM Science color-pHast indicator strips, pH 2-9) using 0.1 M NaOH. The samples were volume-  
25    corrected to 1.150mL with deionized  $H_2O$  and 150  $\mu$ L of 1.0 M NaCl was added to each. The solutions were agitated and optical spectra recorded after 10 min. For a 10 nm colloid, 31.5  $\mu$ g of a-h-IgG ( $F_c$ )/mL of colloid was determined to inhibit aggregation.

To immobilize a-h-IgG ( $\gamma$ ) (and other proteins) on the Au film, the Au surface was modified with MPA as described above in order to introduce carboxylate groups onto the  
30    Au surface. Formation of an active ester at the Au surface was then achieved by reacting 100  $\mu$ L of a 100 mM, pH 5.5, (1-ethyl-3-(3-(dimethylamino)propyl)carbo-diimide

hydrochloride (EDC) solution with the carboxylated Au surface for 15 minutes. A 50  $\mu$ L aliquot of Sulfo-N-hydroxysuccinimide (S-NHS) (40 mM, pH 7) is then injected into the flow cell to stabilize the reactive surface through displacement of the imide moiety. After 15 minutes of incubation with S-NHS, the cell is rinsed with 10 mL of buffer (85 mM phosphate, pH 7) and a 1.0 mg/mL solution of the protein to be immobilized is injected. The surface is incubated with the protein solution for 30 min and is then washed with another 10 mL of phosphate buffer. Unreacted sites on the surface are then blocked by reaction with a 10 mg/mL solution of bovine serum albumin. After another buffer wash, immunochemical reactions may be performed; typical incubation times for antigen and conjugate solutions range from 5 to 30 minutes. All SPR profiles were acquired as described in Example 1 in buffer to eliminate slight index of refraction differences that may exist between protein solutions.

#### Example 3.

##### 15 DNA Detection.

The following materials and methods were used to obtain the data presented in FIGURE 13.

Trisodium citrate dihydrate, poly(ethylene glycol) bis(3-aminopropyl) terminated (PEG), 16-mercaptohexadecanoic acid (90%) (MHA), 3-mercapto-propionic acid (MPA), ethylenediaminetetraacetic acid (EDTA), and NaOH were obtained from Aldrich.  $\text{HAuCl}_4 \cdot 3\text{H}_2\text{O}$  was obtained from Acros.  $\text{NaH}_2\text{P}_2\text{O}_7$ ,  $\text{Na}_2\text{HPO}_4$ , sodium dodecyl sulfate (SDS, 95%), NaCl, KCl, concentrated HCl,  $\text{HNO}_3$ ,  $\text{H}_2\text{SO}_4$ , and 30%  $\text{H}_2\text{O}_2$  were purchased from J. T. Baker Inc. 3-Mercaptopropylmethyldimethoxysilane (MPMDMS) and 3-aminopropyl-trimethoxysilane (APTMS) were purchased from United Chemical Technologies.  $\text{MgCl}_2$ , spectrophotometric grade  $\text{CH}_3\text{COH}$ , and  $\text{CH}_3\text{OCH}_3$  were obtained from EM Science.  $\text{CH}_3\text{CH}_2\text{OH}$  was purchased from Pharmco. 1-ethyl-3-(3-dimethyl-aminopropyl)carbodiimide (EDC), N-hydroxysulfosuccinimide (NHS), and streptavidin were from Pierce. The restriction enzyme Hinf I was purchased from Biolabs. HPLC purified oligonucleotides were purchased from Integrated DNA Technology or from the Pennsylvania State University Nucleic Acid Facility (Chart I). All reagents were used as received without further purification.  $\text{H}_2\text{O}$  used was distilled and subsequently purified

using a Barnstead Nanopure system. Hybridization buffer was prepared with 0.3 M NaCl in a 10-mM phosphate (pH 7.0) buffer. 10  $\mu$ M non-complementary 12-mer oligonucleotides were added as the blocking reagent. 25-mM Tris-HCl (pH 7.8), 100-mM KCl, 10-mM  $MgCl_2$  were mixed and used as the enzyme buffer. Au (99.99%) shots and Cr wires used for evaporation were obtained from Johnson-Matthey Corp. SF11 glass slides (Schott Glass Technologies,  $n=1.78$ ) were used in the SPR scanning experiments, and Fisher Precleaned microscope slides (BK7,  $n=1.515$ ) were used in the imaging experiments.

DNA: Au conjugate preparation. 12-nm diameter colloidal Au was prepared by citrate reduction of  $HAuCl_4 \cdot 3H_2O$  as described in Example 1. Average particle diameters were determined by transmission electron microscopy (TEM), which showed a standard deviation less than 10%. Optical spectra of colloidal Au solutions were recorded using a HP 8453 spectrophotometer.

Thiol-labeled DNA: Au conjugates were prepared according to protocols described in Mirkin *et al.*, Nature 382: 607-609 (1996), Elghanian *et al.*, Science 277:1078-1081 (1997), Storhoff *et al.*, J. Am. Chem. Soc. 120:1959-1964 (1998), Storhoff & Mirkin, Chem. Rev. 99:1849-1862 (1999), and Mucic *et al.*, J. Am. Chem. Soc. 120: 12674-12675 (1998), each of which is incorporated herein by reference in its entirety. 36  $\mu$ M of 12-mer (100  $\mu$ M) oligonucleotide probe S3 was added to 1-ml Au colloid solution. After standing for 16 hrs, the solution was aged in a 0.1 M NaCl solution (pH 7, 10-mM phosphate buffer) for 2 days. The DNA: Au conjugate was then washed by centrifugation (45 min, 12,500 x g) to remove excess reagents. The supernatant was disposed, followed by washing the red pellet with 0.1 M NaCl. After a second centrifugation, the pellet was brought to the original concentration in a 0.3 M NaCl/phosphate hybridization solution. The conjugates were used freshly as prepared, and an optical spectrum was always taken to ensure consistent solution concentration.

Biotinylated DNA: Au conjugates can be prepared from streptavidin: Au conjugate. A solution of Au particles diluted 1:1 in  $H_2O$  and adjusted to pH 8.5 with 0.1 M NaOH was added to 40 RI of 1 mg/ml streptavidin stock solution. After incubating on ice for 1 hr, the solution was centrifuged (12,500 x g, 45 min) to separate unbound protein. 200  $\mu$ L of a biotinylated oligo probe (10  $\mu$ M) was then incubated with the conjugate for 30 min

followed by a second centrifugation with removal of the supernatant and resuspension into hybridization buffer. Again, an optical spectrum was taken to ensure consistent solution concentration as performed with the thiol-labeled DNA conjugates.

Successful incorporation of oligonucleotide probes onto the surface of Au colloid was verified using a method described in Mirkin *et al.*, Nature 382: 607-609 (1996), Elghanian *et al.*, Science 277:1078-1081 (1997), Storhoff *et al.*, J. Am. Chem. Soc. 120:1959-1964 (1998), and Storhoff & Mirkin, Chem. Rev. 99:1849-1862 (1999). In short, S3:Au conjugate solutions were mixed with a linking oligonucleotide that can hybridize to two different copies of S3, and then flocculation induced by the linking oligonucleotide was monitored. While the optical spectrum of the mixture exhibited the characteristic absorbance of Au colloid at 524 nm, the addition of a linking oligonucleotide led to a redshift of  $\lambda_{\max}$ , accompanied by a significant decrease in intensity. This is due to the formation of nanoparticle aggregates. By gradually increasing the solution temperature above the melting point of the DNA duplex, dehybridization occurred and resulted in the dissociation of the colloidal Au network. Consequently, an increase in the optical intensity at 260 nm, a signature absorbance of free oligonucleotides in solution, was observed. DNA:Au conjugates which did not show reversible flocculation in this test were discarded.

Au surfaces were prepared as detailed in Example 1. A self-assembled monolayer was affixed to the Au surface through an overnight immersion in a 10-mM MHA/C<sub>2</sub>H<sub>5</sub>OH solution. An amine-labeled 12-mer oligonucleotide (S1), with a sequence complementary to half of the target S2, was coupled to the carboxylate groups on the surface via EDC/NHS cross-linking. Amine-labeled PEG (1 %) was then introduced to block unreacted sites, followed by rinsing and the incubation of the target analyte, a 24-mer DNA (S2), in hybridization buffer for 2 hrs. In the unamplified experiment, an untagged DNA probe (S3), with sequence complementary to the other half of S2, was added and incubated with surface. In the amplified event, however, the SPR surface was exposed to the Au particle-tagged S3 probes. In both cases, hybridization was carried out for 1 hr, followed by extensive rinsing with a 0.2% SDS/0.1 M NaCl buffer.

Scanning SPR data was acquired using the instrument as described in Example 1. A miniature peristaltic pump (Intech Laboratories, Inc.) was used to deliver analyte

solutions to the sample cell at 0.1 ml/min. A 5-min H<sub>2</sub>O rinse at 1 ml/min was always carried out before collecting SPR measurements. All experiments were completed at room temperature except for DNA melting, in which the temperature of the sample cell was increased by flowing warm dehybridization buffer (80 °C as measured at the water bath) for 20 min. A much higher temperature, 27 °C above the melting point of the surface-confined DNA duplex, was applied here due to thermal gradients in the liquid delivery apparatus. The actual temperature at the surface is estimated to be between 60 and 70° C. The sample cell was cooled down to room temperature before the SPR measurement. Kinetic studies were carried out by monitoring SPR reflectivity changes as a function of incubation time at a fixed angle (53.2°).

Imaging SPR was carried out using the instrument described above. Data were plotted as spatial intensity maps of the SPR substrate surface, where an increase in intensity indicates an increase in SPR response. A commercial software package, NIH Image, was used for image analysis. From the spatial intensity map the integrated intensity from each sample cell was calculated, a baseline intensity was subtracted, and each signal was normalized for the area of the sample cell.

UV-Vis Absorbance Spectroscopy: UV-vis spectra were collected using a HP 8453 diode array spectrophotometer equipped with a HP 89090A Peltier temperature controller. By changing the solution temperature from 25-65 °C at 1 °C/step, a DNA melting assay was tested by monitoring the optical intensity changes at 260 nm. Hybridization buffer was used as the blank.

#### Example 4.

##### Wet Chemical Synthesis of Thin Au Films.

Glass coverslips ( $n = 1.515$ , Fisher) were washed by immersion in a 'piranha' bath (30% H<sub>2</sub>O<sub>2</sub> mixed in a 1:4 ratio with concentrated H<sub>2</sub>SO<sub>4</sub>. Caution should be used in handling this solution as it is extremely oxidizing). The clean glass slides were then functionalized with a self assembled mono-layer of (3-mercaptopropyl)methyl-dimethoxysilane (MPMDMS, United Chemical Technologies) by exposure to a 1-10 mM ethanolic solution of the silane for 30 minutes. A functionalized slide was then placed in a 17 nM solution of 12 nm diameter colloidal Au until a surface coverage that yielded an absorbance of 0.1 AU at 520 nm was obtained. The colloidal Au-modified surface was

then placed in 500 mL of aqueous 0.5 mM  $\text{NH}_2\text{OH}\cdot\text{HCl}$  (Aldrich), to which 100 mL of 0.06%  $\text{HAuCl}_4$  (Acros) was added while agitating on an orbital shaker at 150 revs/minute. Agitation was continued for 20 minutes to produce a smooth, reflective Au surface on the monolayer.

5

Example 5.

Synthesis of PDMS Microwell Array.

Film thicknesses were determined by measuring the step height at a scribed spot on the surface via tapping-mode atomic force microscopy (TM-AFM) as described in

10 Example 1 using standard 200  $\mu\text{m}$  etched silicon probes, an acquisition frequency of 1.5Hz, and line density of 512.

PDMS (Dow Corning Sylgard 184 in a 10:1 ratio of elastomer to hardener) is mixed, degassed using a vacuum dessicator, and poured over a one inch square electronic breadboard master into a small petri dish. This composite is degassed using a vacuum  
15 dessicator and then cured overnight in a 50° C oven. After cooling, the new PDMS “master” is peeled away from the electronic breadboard. This new “master” is used to form the final mold of PDMS. Additional PDMS is then poured in between the new master and the petri dish, degassed, and cured in an oven overnight. An aluminum block, attached to a glass microscope slide is placed on top as a weight to assure constant contact  
20 with the bottom of the petri dish. This PDMS sandwich is removed from the oven, cooled, and then peeled apart revealing the PDMS replica of the electronic breadboard.

## CLAIMS:

1. A microwell array comprised of a plurality of spatially discrete microvolume wells, wherein said array is comprised of PDMS.  
5
2. The microwell array of claim 1 comprised of between 10 and 200 wells.
3. The microwell array of claim 1 wherein said array is associated with a thin metal film which serves as the bottom surface of said plurality of wells.  
10
4. The microwell array of claim 3 wherein said thin metal film is a surface plasmon resonance active metal.
5. The microwell array of claim 4 wherein said thin metal film is selected  
15 from the group consisting of Au, Ag, Al and Cu.
6. The microwell array of claim 3 wherein said thin metal film is coated on a glass surface.
- 20 7. A method for associating a plurality of reagents on spatially discrete regions of a surface comprising:  
providing a microwell array template on the surface, wherein said microwell array is comprised of PDMS, and wherein the array provides a plurality of spatially discrete wells and the bottom of each of the wells is a region of said surface;  
25 introducing reagents into said wells that associate with the surface; and removing said template.
8. The method of claim 7 wherein said surface is a thin metal film.
- 30 9. The method of claim 8 wherein said thin metal film is a surface plasmon resonance active metal.



10. The method of claim 9 wherein said thin metal film is selected from the group consisting of Au, Ag, Al and Cu.

11. The method of claim 8 wherein said thin metal film is coated on a glass surface.

12. A method for conducting an assay for an analyte in a test solution that may contain said analyte comprising: providing a surface plasmon resonance active surface; associating a molecule with said surface, wherein said molecule is associated with a colloidal metal nanoparticle; contacting said surface with said test solution, wherein the presence or absence of said analyte changes the relative distance between the surface and said nanoparticle; and detecting said distance by measuring the SPR profile.

13. The method of claim 12 wherein said surface plasmon resonance active surface is a thin metal film.

14. The method of claim 13 wherein said thin metal film is selected from the group consisting of Au, Ag, Al and Cu.

15. The method of claim 13 wherein said thin metal film is coated on a glass surface.

16. The method of claim 12 wherein said colloidal metal nanoparticle is comprised of a metal selected from the group consisting of Au, Ag, Al and Cu.

17. The method of claim 12 wherein said colloidal metal nanoparticles are substantially spherical.

18. The method of claim 17 wherein said colloidal metal nanoparticles are 1 nm to 150 nm in diameter.

19. A method for conducting a plurality of assays for a plurality of analytes in a test solution that may contain said analytes comprising:

- 5 providing a surface plasmon resonance active surface; associating a plurality of ligands to said analytes to said surface;
- contacting said surface with said test solution, wherein the presence or absence of an analyte results in a specific type of colloidal metal nanoparticle associating with a specific type of ligand at or near said surface; and
- 10 detecting for said association between said specific type of ligand and said specific type of colloidal metal nanoparticle by measuring the SPR profile, wherein the SPR profile is distinguishable between the different types of colloidal metal nanoparticles.

20. The method of claim 19 wherein the types of colloidal metal nanoparticles are distinguished by their size.

15

21. The method of claim 19 wherein the types of colloidal metal nanoparticles are distinguished by their composition.

22. The method of claim 19 wherein said surface plasmon resonance active surface is a thin metal film.

20

23. The method of claim 22 wherein said thin metal film is selected from the group consisting of Au, Ag, Al and Cu.

24. The method of claim 22 wherein said thin metal film is coated on a glass surface.

25

25. The method of claim 19 wherein said colloidal metal nanoparticle is comprised of a metal selected from the group consisting of Au, Ag, Al and Cu.

30

26. The method of claim 19 wherein said colloidal metal nanoparticles are substantially spherical.

27. The method of claim 26 wherein said colloidal metal nanoparticles are 1 nm to 150 nm in diameter

5 28. A method for conducting an assay for an analyte in a test solution that may contain said analyte comprising:

providing a surface plasmon resonance active surface;

conducting said assay at or near said surface, wherein the presence or absence of a colloidal metal nanoparticle indicates the presence or absence of said analyte  
10 in said test solution;

detecting said presence or absence of said nanoparticle by measuring the SPR profile of said surface with an interferometer SPR.

29. The method of claim 28 wherein said surface plasmon resonance active  
15 surface is a thin metal film.

30. The method of claim 29 wherein said thin metal film is selected from the group consisting of Au, Ag, Al and Cu.

20 31. The method of claim 29 wherein said thin metal film is coated on a glass surface.

32. The method of claim 28 wherein said colloidal metal nanoparticle is comprised of a metal selected from the group consisting of Au, Ag, Al and Cu.

25

33. The method of claim 28 wherein said colloidal metal nanoparticles are substantially spherical.

34. The method of claim 33 wherein said colloidal metal nanoparticles are 1  
30 nm to 150 nm in diameter.

35. A method for conducting an assay for an analyte in a test solution that may contain said analyte comprising:

providing a surface plasmon resonance active surface;

conducting said assay at or near said surface,

5 wherein the present absence of a colloidal metal nanoparticle indicates the presence or absence of said analyte in said solution, and wherein said colloidal metal nanoparticle is comprised of an AuS/Au shell particle; and

detecting said presence or absence of said nanoparticle by measuring the SPR profile of said surface.

10

36. The method of claim 35 wherein said surface plasmon resonance active surface is a thin metal film.

37. The method of claim 36 wherein said thin metal film is selected from the  
15 group consisting of Au, Ag, Al and Cu.

38. The method of claim 36 wherein said thin metal film is coated on a glass surface.

20 39. The method of claim 35 wherein said colloidal metal nanoparticle is comprised of a metal selected from the group consisting of Au, Ag, Al and Cu.

40. The method of claim 35 wherein said colloidal metal nanoparticles are substantially spherical.

25

41. The method of claim 40 wherein said colloidal metal nanoparticles are 1 nm to 150 nm in diameter.

42. A method for high-throughput screening of combinatorial libraries to  
30 identify compounds having a positive response for a preselected activity, comprising:  
providing a surface plasmon resonance active surface;

contacting a plurality of screening assays on said surface whereby a plurality of members of said combinatorial library are associated with said surface, and wherein a positive response for said preselected activity is associated with the presence or absence of a colloidal metal nanoparticle with said surface; and

- 5                    detecting said presence or absence of said nanoparticle by measuring the SPR profile of said surface to identify compounds having a positive response for said preselected activity.

43.     The method of claim 42 wherein said surface plasmon resonance active  
10    surface is a thin metal film.

44.     The method of claim 43 wherein said thin metal film is selected from the group consisting of Au, Ag, Al and Cu.

- 15           45.     The method of claim 43 wherein said thin metal film is coated on a glass surface.

46.     The method of claim 42 wherein said colloidal metal nanoparticle is comprised of a metal selected from the group consisting of Au, Ag, Al and Cu.

20

47.     The method of claim 42 wherein said colloidal metal nanoparticles are substantially spherical.

48.     The method of claim 47 wherein said colloidal metal nanoparticles are 1  
25    nm to 150 nm in diameter.

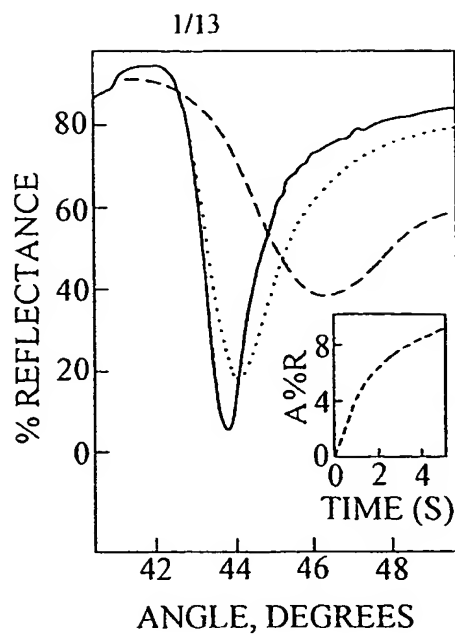


FIG. 1

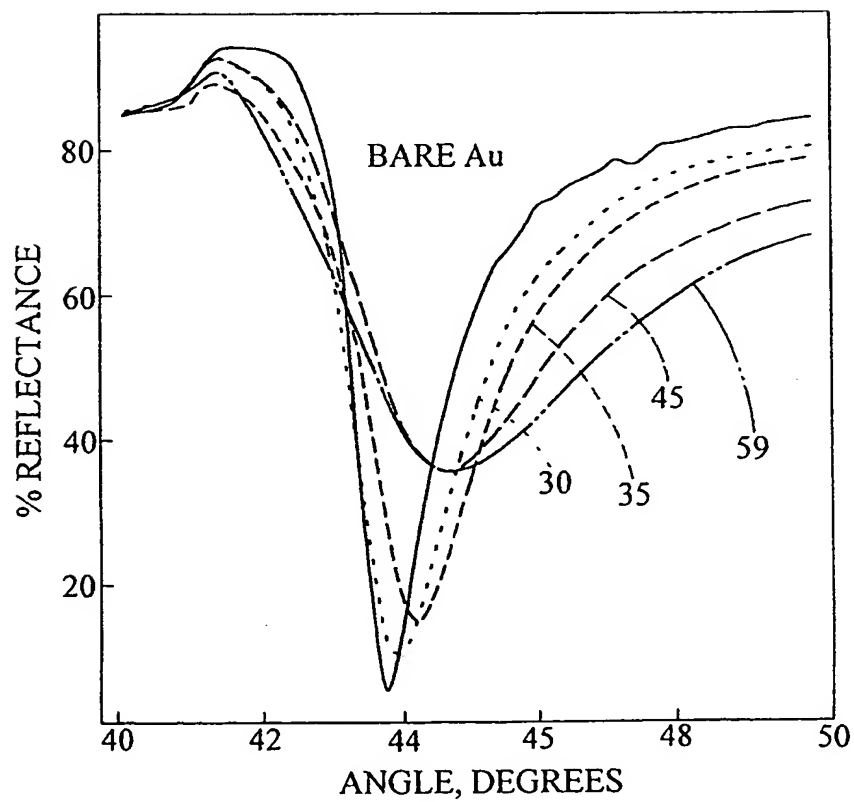


FIG. 2

2/13

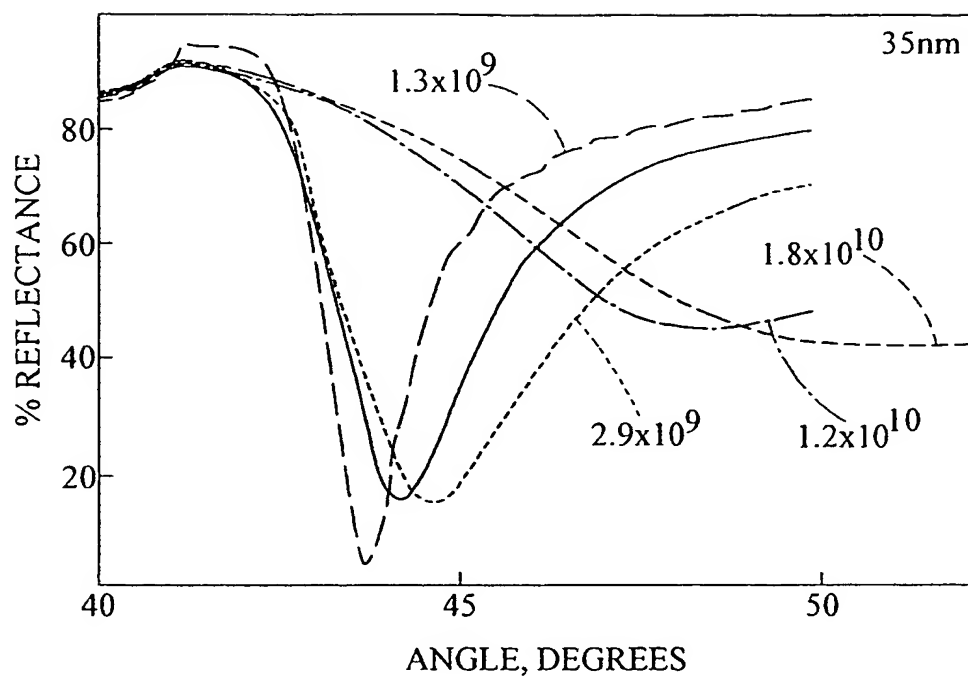


FIG. 3A

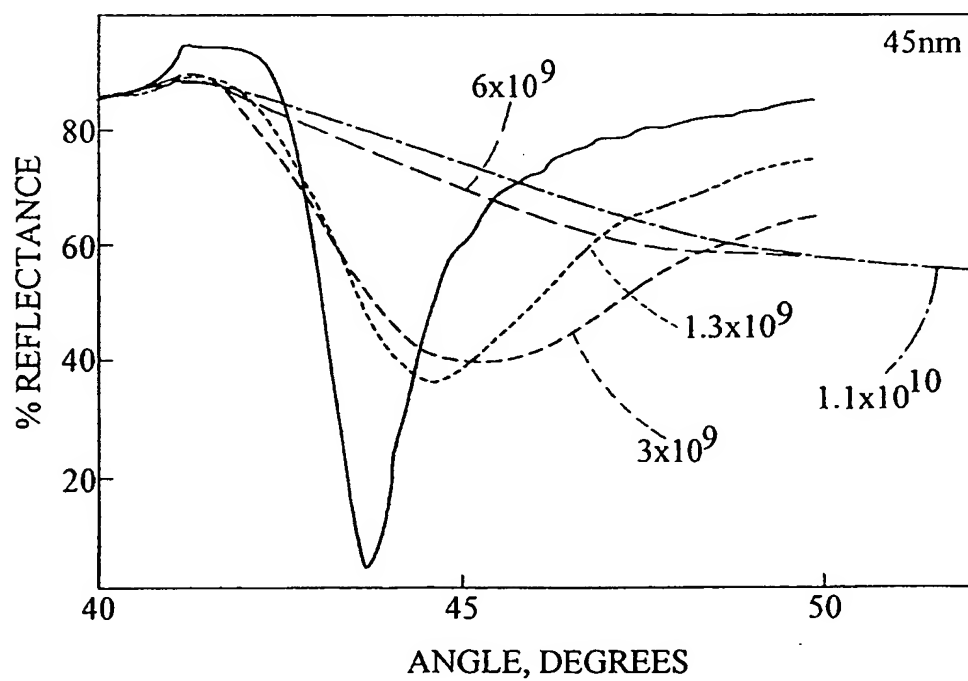


FIG. 3B

3/13

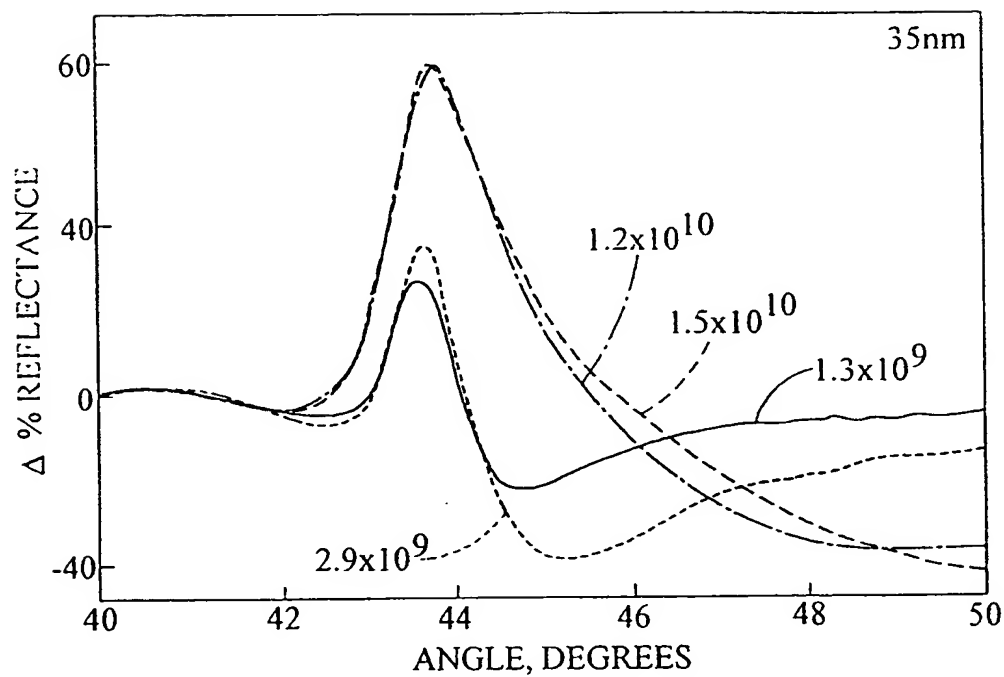


FIG. 4A

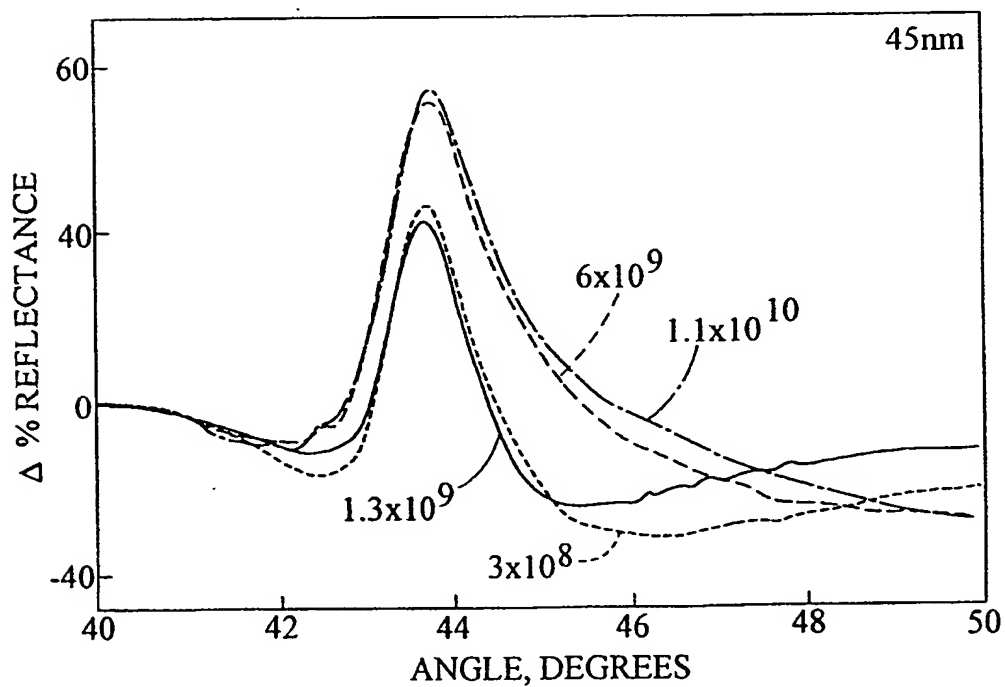


FIG. 4B



4/13


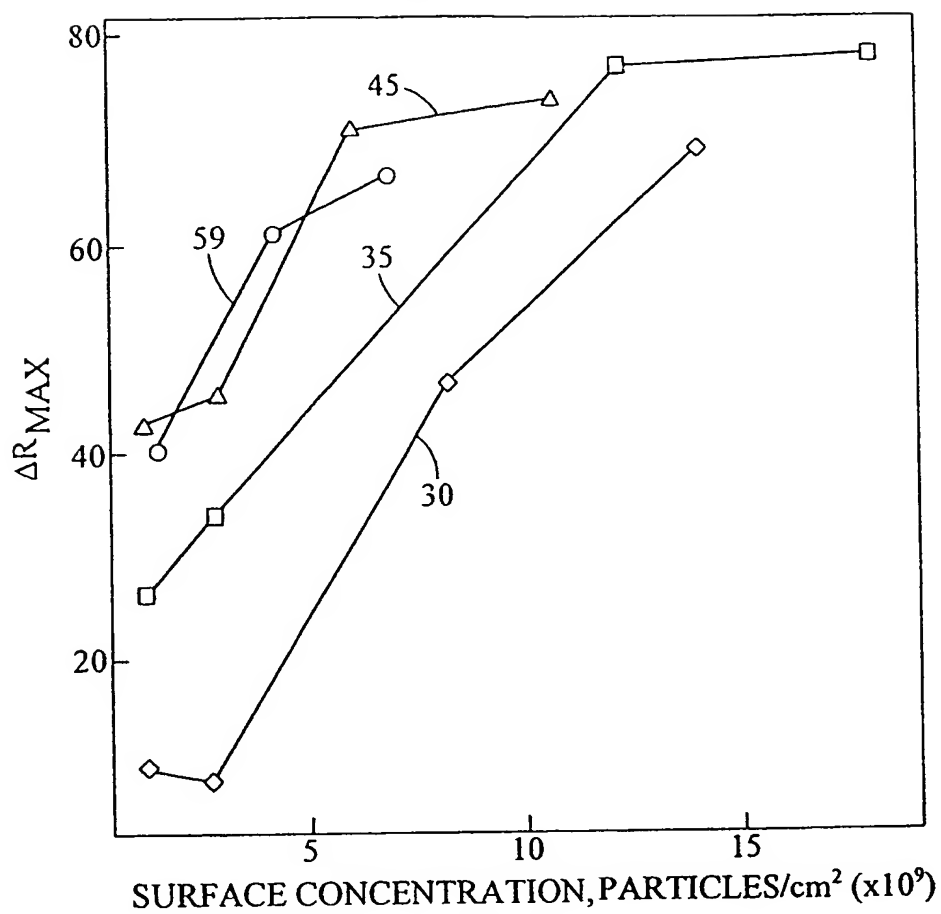


FIG. 5

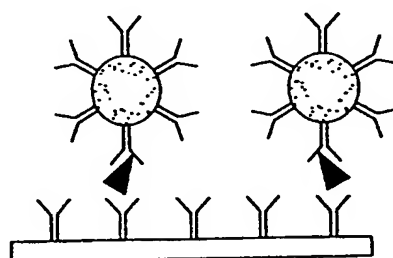

▼ = ANTIGEN

● = Au COLLOID

Y = ANTIBODY

FIG. 6

5/13

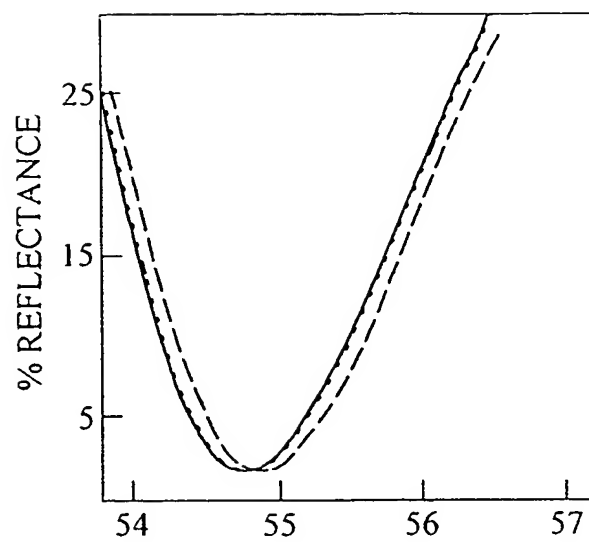


FIG. 7A

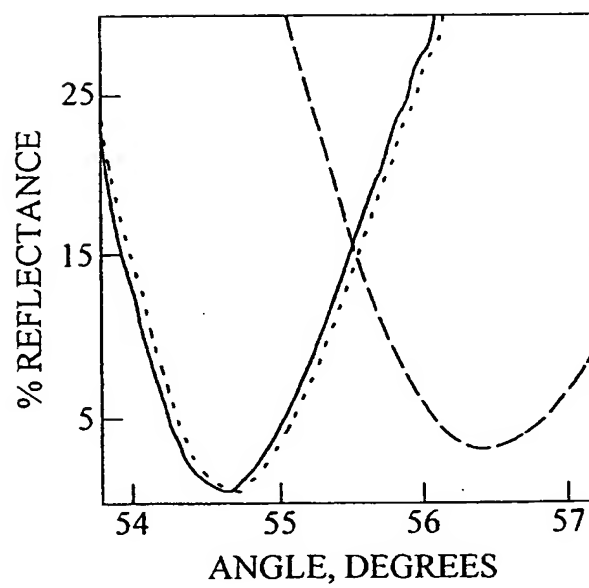


FIG. 7B

6/13

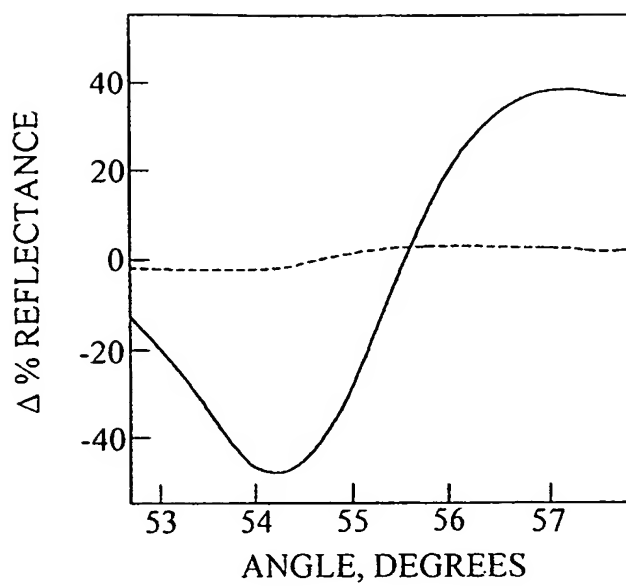


FIG. 8

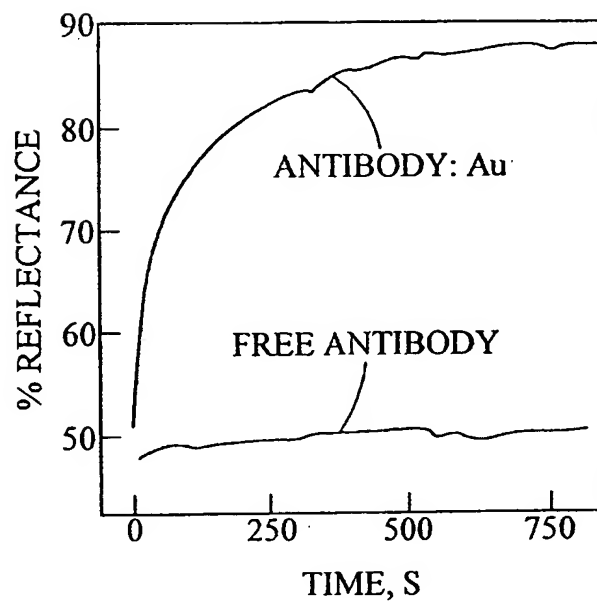


FIG. 9

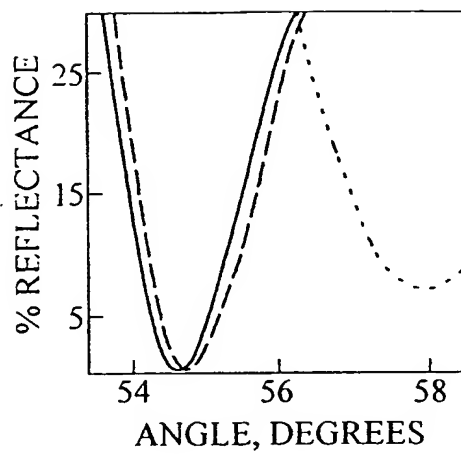


FIG. 10A

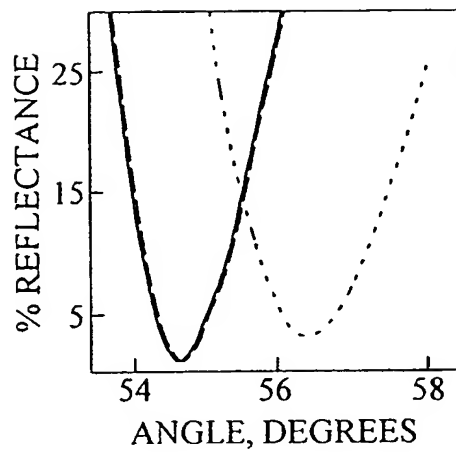


FIG. 10B

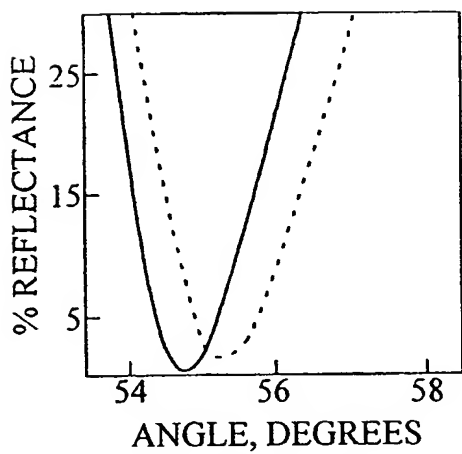


FIG. 10C

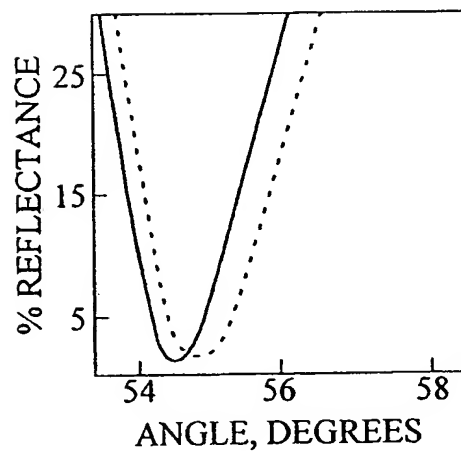


FIG. 10D

8/13

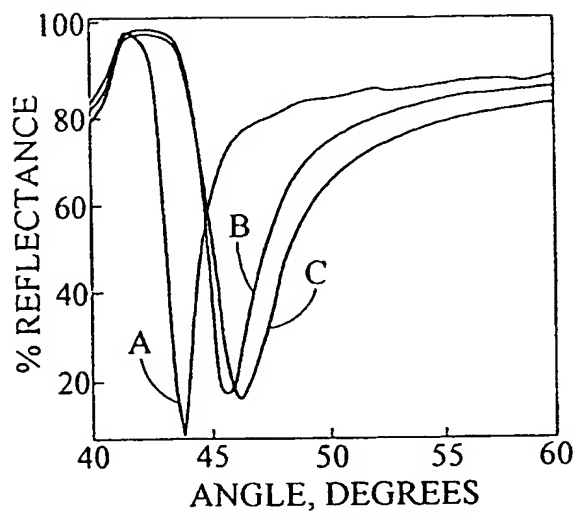


FIG. 11A

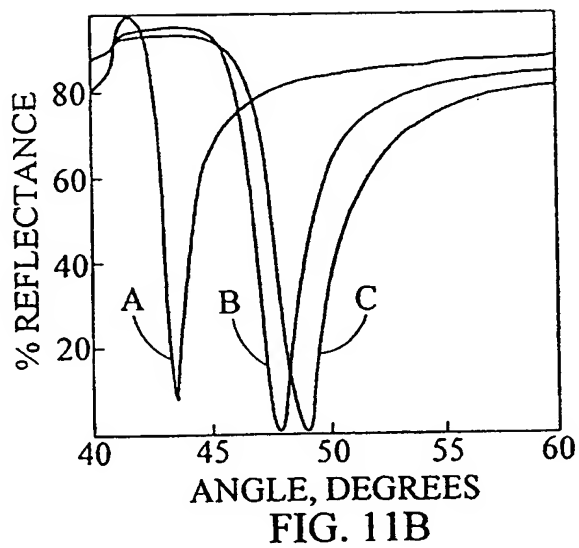


FIG. 11B

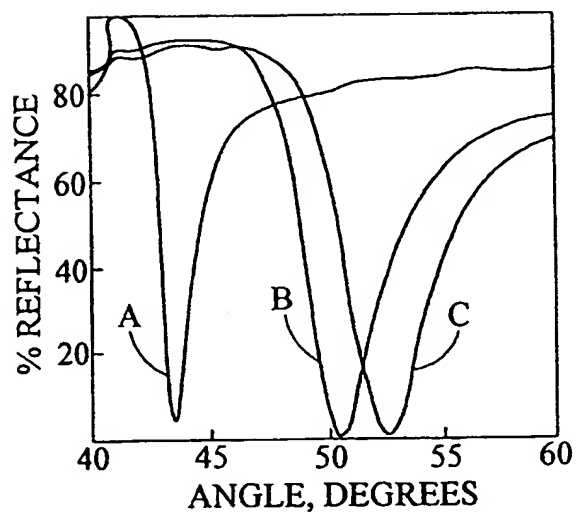


FIG. 11C

9/13

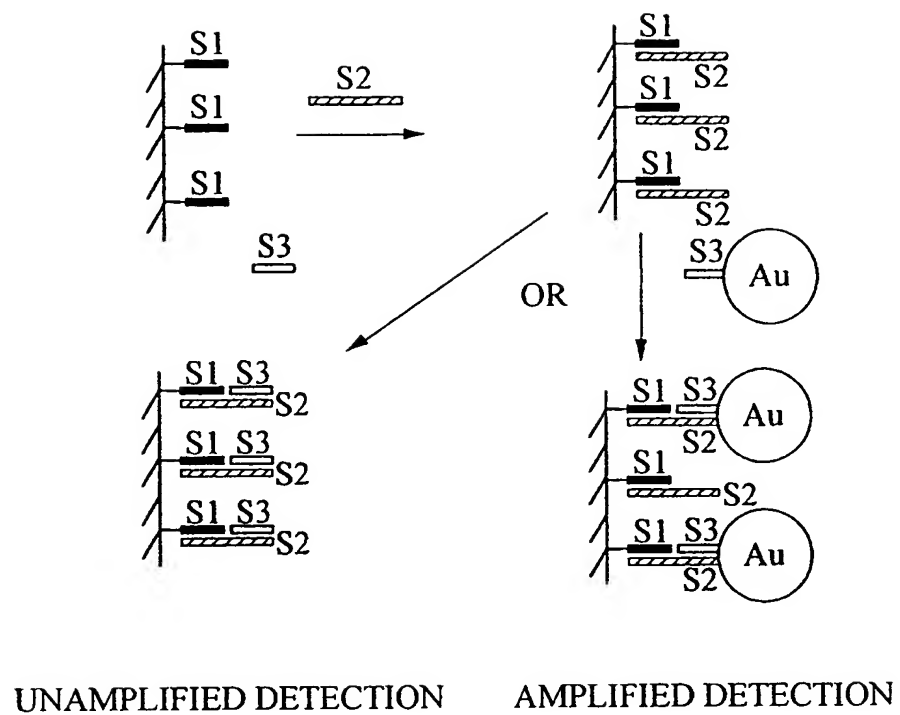


FIG. 12

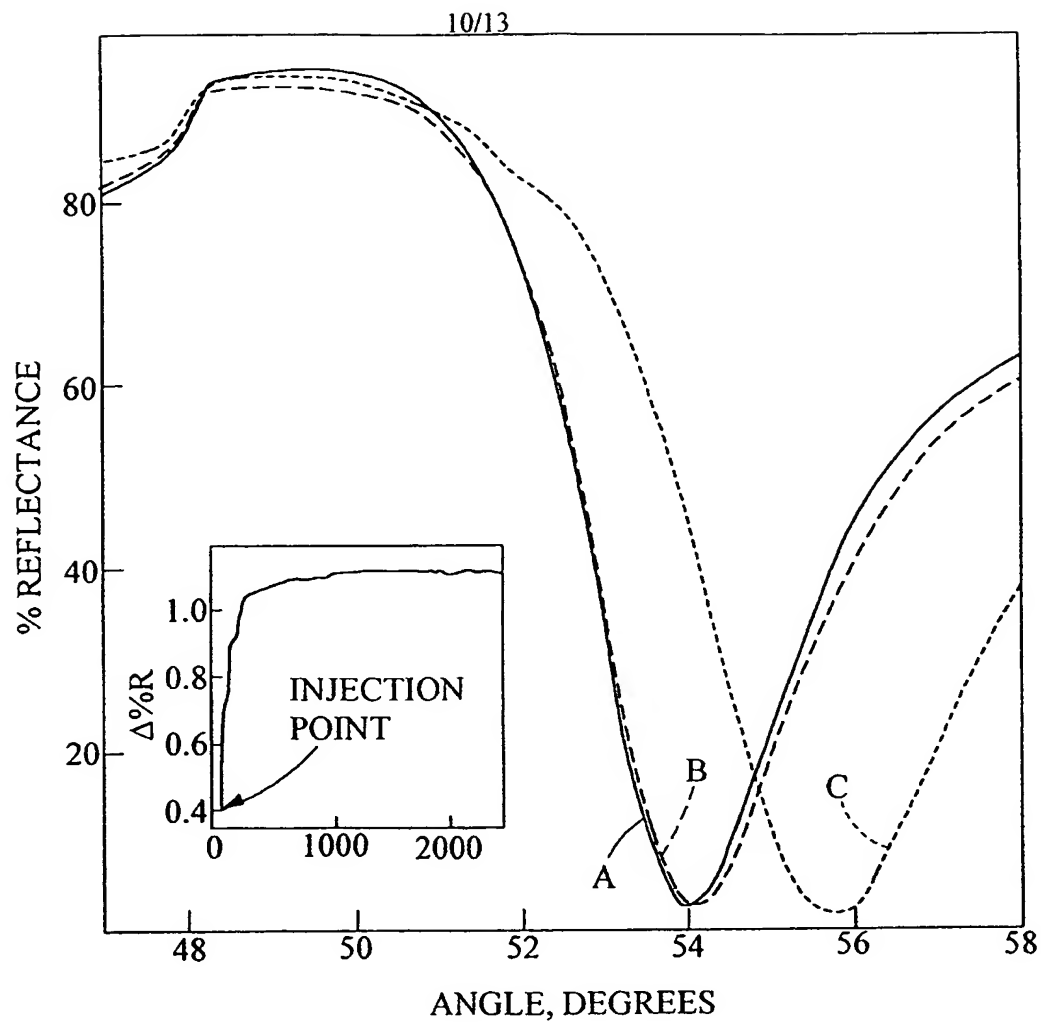


FIG. 13

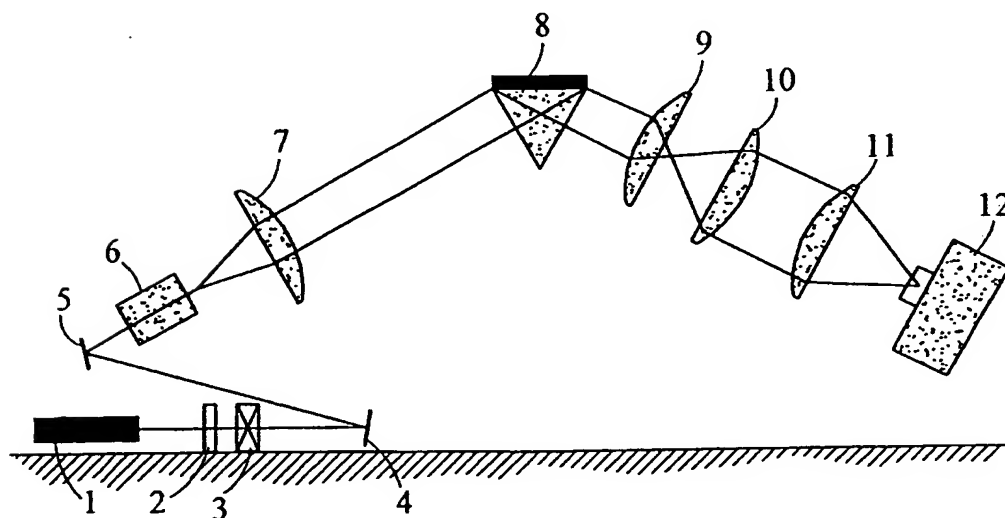


FIG. 14

11/13

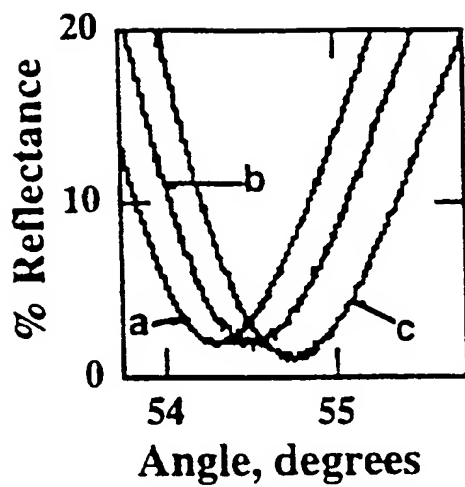


Fig. 15A

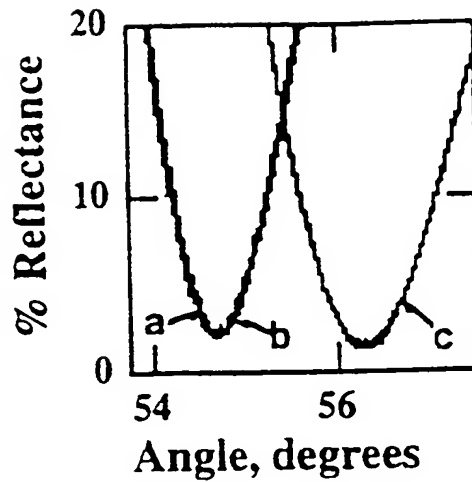


Fig. 15B

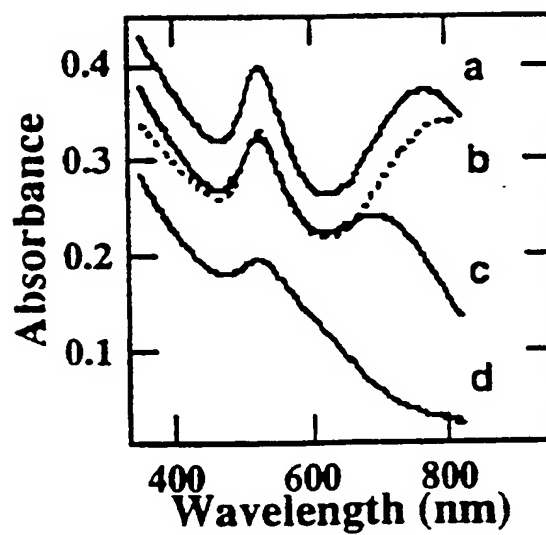


Fig. 16



12/13

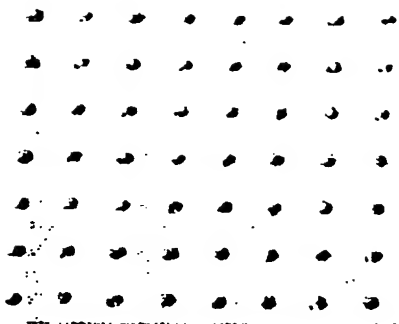


Fig. 17A

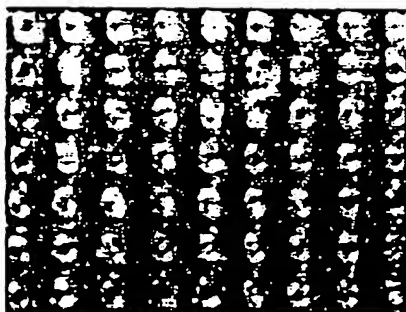


Fig. 17B

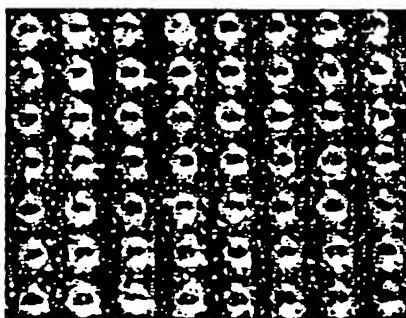


Fig. 17C

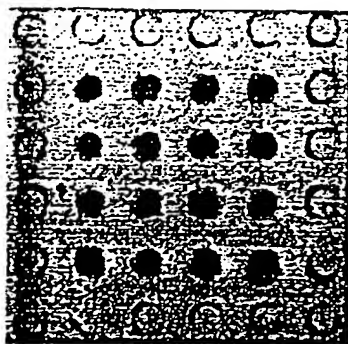


Fig. 18A

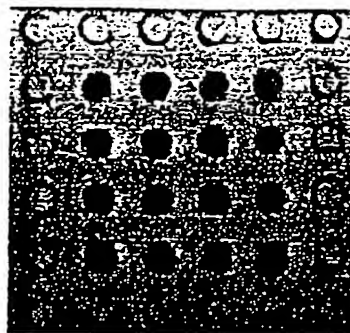


Fig. 18B

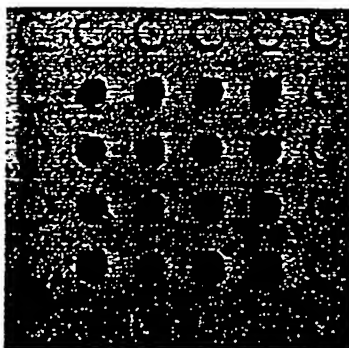


Fig. 18C

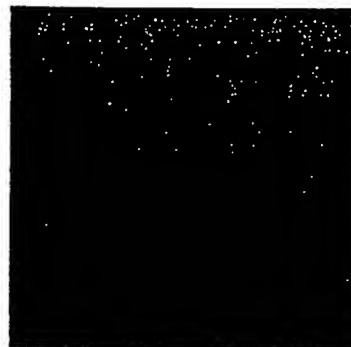


Fig. 18D

## INTERNATIONAL SEARCH REPORT

International application No.

PCT/US00/42139

## A. CLASSIFICATION OF SUBJECT MATTER

IPC(7) : G01N 21/65

US CL : 422/82.05, 102; 436/525, 164; 356/301

According to International Patent Classification (IPC) or to both national classification and IPC

## B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)

U.S. : 422/82.05, 102; 436/525, 164; 356/301

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Electronic data base consulted during the international search (name of data base and, where practicable, search terms used)

EAST

search terms microwell, PDMS, surface plasmon resonance, colloidal metal nanoparticle

## C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
X,P	US 6,068,752 A (DUBROW et al) 30 May 2000, figs. 3-5, col. 6, lines 22-60.	1,2
Y	US 5,609,907 A (NATAN) 11 March 1997, entire document.	12-18, 28-34
X,E	US 6,149,868 A (NATAN et al) 21 November 2000, entire document.	12-48

☐ Further documents are listed in the continuation of Box C.
 ☐ See patent family annex.

* Special categories of cited documents:	*T* later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention
*A* document defining the general state of the art which is not considered to be of particular relevance	*X* document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone
*E* earlier document published on or after the international filing date	*Y* document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art
*L* document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)	*A* document member of the same patent family
*O* document referring to an oral disclosure, use, exhibition or other means	
*P* document published prior to the international filing date but later than the priority date claimed	

Date of the actual completion of the international search

03 APRIL 2001

Date of mailing of the international search report

27 APR 2001

 Name and mailing address of the ISA/US  
 Commissioner of Patents and Trademarks  
 Box PCT  
 Washington, D.C. 20231

Facsimile No. (703) 305-3230

Authorized officer

DWAYNE HANDY

Telephone No. (703) 308-0661

**This Page is Inserted by IFW Indexing and Scanning  
Operations and is not part of the Official Record**

**BEST AVAILABLE IMAGES**

Defective images within this document are accurate representations of the original documents submitted by the applicant.

Defects in the images include but are not limited to the items checked:

- ☐ BLACK BORDERS
- ☐ IMAGE CUT OFF AT TOP, BOTTOM OR SIDES
- ☐ FADED TEXT OR DRAWING
- ☒ BLURRED OR ILLEGIBLE TEXT OR DRAWING
- ☐ SKEWED/SLANTED IMAGES
- ☐ COLOR OR BLACK AND WHITE PHOTOGRAPHS
- ☐ GRAY SCALE DOCUMENTS
- ☒ LINES OR MARKS ON ORIGINAL DOCUMENT
- ☐ REFERENCE(S) OR EXHIBIT(S) SUBMITTED ARE POOR QUALITY
- ☐ OTHER: \_\_\_\_\_

**IMAGES ARE BEST AVAILABLE COPY.**

**As rescanning these documents will not correct the image problems checked, please do not report these problems to the IFW Image Problem Mailbox.**